




Product Catalog  
CONOLOG<sup>®</sup> Implant System

Valid from August 2023



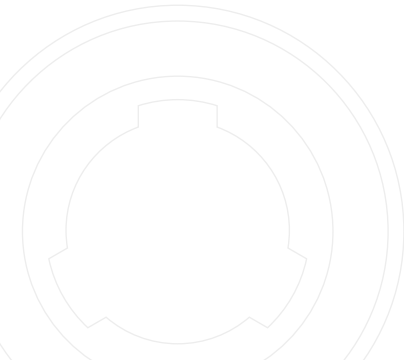

# Content

## Service

---

Clinical evidence and Science	2
-------------------------------	---

## System information

---

The CONELOG® Implant System	3
-----------------------------	---

## Surgery

---

Planning	18
PROGRESSIVE-LINE Implants and Instruments	20
PROGRESSIVE-LINE Guide System Instruments	26
PROGRESSIVE-LINE Flex Instruments	33
SCREW-LINE Implants and Instruments	37
SCREW-LINE Guide System Instruments	45
General Surgical Instruments	48
SCREW-LINE Osteotomy Sets	57
Cover Screws	62
Healing Caps	62

## Prosthetics

---

Scanbody	64
Impression Taking	65
Bite Registration	66
Cast Fabrication	66
Temporary Abutments	67
CAD/CAM Prosthetics	68
CAM Blanks	70
Esthomic® Abutments	72
Universal Abutments	74
Gold-plastic Abutment	74
COMFOUR® System	76
Ball Abutment Anchoring System	81
Locator® Anchoring System	82
Double Crown Restoration	87
Accessories for Abutments	87
Prosthetic Instruments	88
Instruments for Dental Technicians	92
Selection Abutments	93

## Auxiliary Articles

---

Implants for Practice	96
Insertion Posts	96
Demonstration Models	97
Macro Models	97
Literature	98

## Additional Information

---

Indication Overview	102
Implant Overview	104
Prosthetic Overview	106
Screw Overview	112, 114
Overview Auxiliary Screws	113
Overview Tightening Torques	116
Materials	118

## Index

---

Alphabetical	120
Article Number	124

## Further Information

---

Further Documentation	136
Legal	136

# Clinical evidence and Science

From the beginning on, the Camlog company has set high standards in scientific documentation of all essential properties of their implant systems.

In **Clinical evidence and Science**, we have summarized the current state of research on Camlog Implant Systems.

We are happy to pass on this concentrated knowledge to you. You are also welcome to request printed version.



[www.biohorizonscamlog.com/clinical-evidence-and-science](http://www.biohorizonscamlog.com/clinical-evidence-and-science)



# The CONELOG® Implant System



The CONELOG® Implant System is based on years of clinical and laboratory experience and is a user-friendly, prosthetically oriented implant system.

All CONELOG® Products are manufactured with the latest state-of-the-art technology. The CONELOG® Implant System is continuously developed by the company's research and development team in collaboration with clinics, universities and dental technicians and therefore stays abreast of the latest technology.

The CAMLOG® and CONELOG® Implant Systems are very well documented scientifically. Studies\* support this with respect to many parameters including the implant surface, time of implantation and/or implant loading, primary stability, and the connection design.

\* See "Further documentation" on page 136

## CONELOG® PROGRESSIVE-LINE Implants

The CONELOG® PROGRESSIVE-LINE Implants make it easier to implement modern treatment concepts such as immediate restorations or immediate loading, which require high primary stability [1, 2]\*.

The geometry of the implant is consistently designed to develop high initial stability:

- The self-tapping screw implant has a conically shaped apical area that enables pronounced primary stability even in soft bone [1, 2]\*.
- Thread extending to the apex for good anchorage in immediate implantations [1, 2]\*.
- Crestal thread for improved hold with limited bone height [2]\*.

CONELOG® PROGRESSIVE-LINE Implants are available with the Promote® plus Surface which extends over the entire implant body up to the acid-etched conical 45° implant shoulder. Depending on the clinical situation, this surface design thus permits slightly subcrestal implant positioning in the sense of a classic bone level implant.

CONELOG® PROGRESSIVE-LINE Implants with screw-mounted insertion post can be used for template-guided implant dentistry.


CONELOG® PROGRESSIVE-LINE Implants feature the high-precision, conical CONELOG® Implant-abutment connection with integrated Platform Switching. Prosthetic restoration is performed with CONELOG® Abutments.

\* See "Further documentation" on page 136



CONELOG® PROGRESSIVE-LINE  
Implant, Promote® plus

### Implant diameter

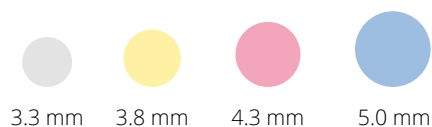

### Implant lengths



### Promote® Surface

CONELOG® Implants are available with the abrasive-blasted, acid-etched Promote® Surface. The surface is based on current scientific knowledge and supports rapid osseointegration. Scientific results from studies with cell cultures, osteohistology and in pull-out trials illustrate this impressively.

## CONELOG® SCREW-LINE Implants

CONELOG® SCREW-LINE Implants are slightly conical, self-tapping screw implants. They enable easy insertion by self-centering with continuous bone contact and thus achieve solid primary stability.

CONELOG® Implants are available with the abrasive-blasted, acid-etched Promote® Surface up to the acid-etched conical 45° implant shoulder and thus allow for maximum flexibility when determining the vertical implant position. Rounding of the apical geometry ensures gentle insertion of the CONELOG® SCREW-LINE Implants into the bone, also near the maxillary sinus.


CONELOG® SCREW-LINE Implants with screw-mounted insertion post can be used for template-guided implant dentistry.

CONELOG® PROGRESSIVE-LINE Implants feature the high-precision, conical CONELOG® Implant-abutment connection with integrated Platform Switching. Prosthetic restoration is performed with CONELOG® Abutments.



**CONELOG® SCREW-LINE  
Implant, Promote® plus**

### Implant diameter

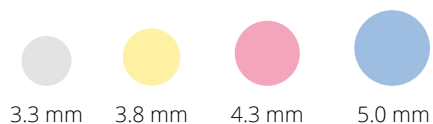

3.3 mm    3.8 mm    4.3 mm    5.0 mm

### Implant lengths




All CONELOG® Implants are delivered pre-assembled in sterile packaging on a color-coded insertion post corresponding to the diameter.



## The insertion posts of the CONELOG® Implants

The PROGRESSIVE-LINE and SCREW-LINE Implants are each offered with two different versions of the insertion post. Regardless of which option you choose, the instruments used to insert the implant are identical. A separate set of instruments for guided surgery is not required.

- Pre-assembled transfer part – simplified application and transfer to the patient's mouth
- Small diameter – easy access to the interdental spaces and posterior region
- Color-coded insertion post according to diameter – provides easy orientation during surgery
- Can be used as a paralleling pin – for aligning the position of multiple implants

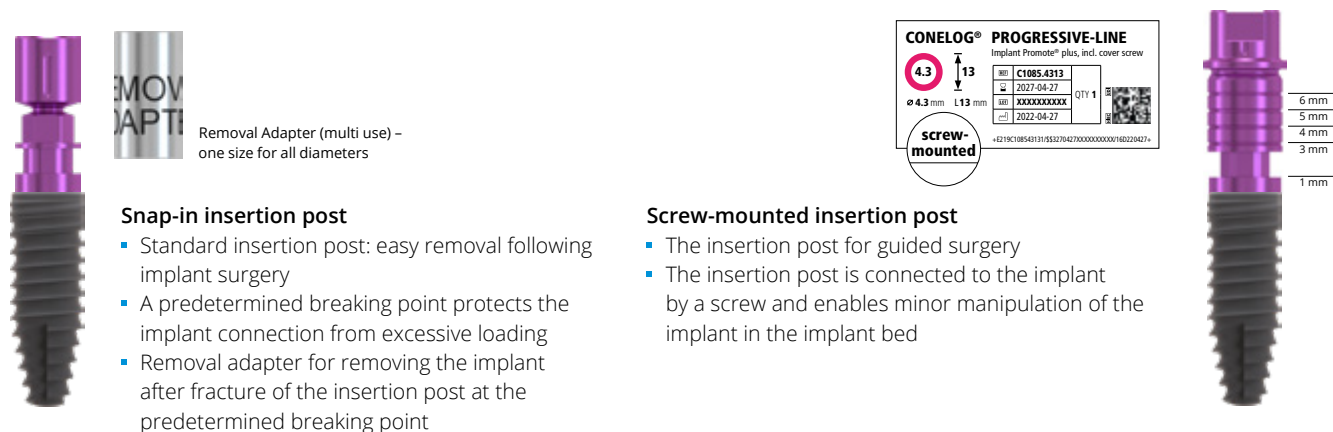

## CONELOG® Implant-abutment connection

The geometry of the CONELOG® Implant-abutment connection enables integrated Platform Switching and provides excellent tactile feedback when inserting the abutments.

Indexing via the three grooves/cams allows the cams to slide noticeably into the grooves of the implant and thus into the final position when the abutment is rotated slightly. Simple, easy and safe orientation in the longitudinal axis of the implant is thus ensured. The precise conical connection minimizes micro-movements and demonstrates superior stability compared to other conical connections [3, 4]\*.


\* See "Further documentation" on page 136.

## Advantages and benefits of the CONELOG® Connection

- Simple, fast and precise abutment positioning with clearly noticeable tactile feedback
- Precise, conical implant-abutment connection with superior stability compared to other conical connections<sup>1,2\*</sup>
- Integrated Platform Switching

For optimal positioning of the abutments, the implant should be aligned in the bone so that one of the three grooves points in vestibular direction. With the CONELOG® Implants, the insertion tools include markings that correspond to the three grooves of the implant inner configuration.

\* See "Further documentation" on page 136.

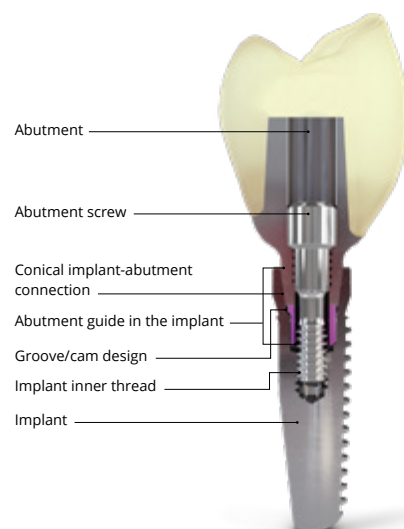



## CONOLOG® Prosthetic components

The CONOLOG® Implants can be provided with a wide range of flexible, anatomically adapted prosthetic components. CONOLOG® Abutments are color-coded according to the implant diameters.

### Effect of the Platform Switching design

The CONOLOG® Implant System offers integrated Platform Switching as the implant shoulder is not covered by the healing caps and abutments. Platform Switching is used to support the hard and soft tissue in the peri-implant esthetic region. The distance between the implant-abutment interface and the alveolar crest is increased and thereby reduces the effect of inflammatory cell infiltration with concomitant bone resorption.



### CONOLOG® Healing caps

CONOLOG® Healing caps sit on the machined implant shoulder, but do not cover it completely. As a result, the soft tissue over the shoulder can be adapted. The conical surfaces do not come into contact.

The healing caps are used according to their indication for single and two-stage procedures. The healing caps are available in three geometries (cylindrical, wide body and bottleneck) and are screwed directly into the implant.

### CONOLOG® Impression taking

Impression-taking of the CONOLOG® Implants is possible with impression posts, open or closed tray. All impression-taking components are color-coded based on the implant diameter. High-precision components ensure correct transfer of the intraoral situation.

The CONOLOG® Impression posts do not lock into the cone of the implant, but lie on the implant shoulder. Thus, a vertical offset is prevented when taking the impression. The antirotational mechanism is ensured by the CONOLOG® groove/cam geometry.





### CONELOG® Temporary abutments


CONELOG® Temporary abutments made of titanium alloy are available for temporary restorations in crown and bridge versions. The abutments can be used in immediate implantations or after exposing the gingiva.

### CONELOG® Esthomic® Abutments

Anatomically preformed abutments allow for optimal stump design. The CONELOG® Esthomic® Abutments are available both straight and angled with various gingival heights and with an oval anatomically pre-shaped shoulder profile. The angled Esthomic® Abutments are available in A and B versions differentiated by a cam offset of 60°. This results in six prosthetic-oriented rotating positions and allows perfect prosthetic alignment of the axes.



### CONELOG® Esthomic® Abutment cam alignment

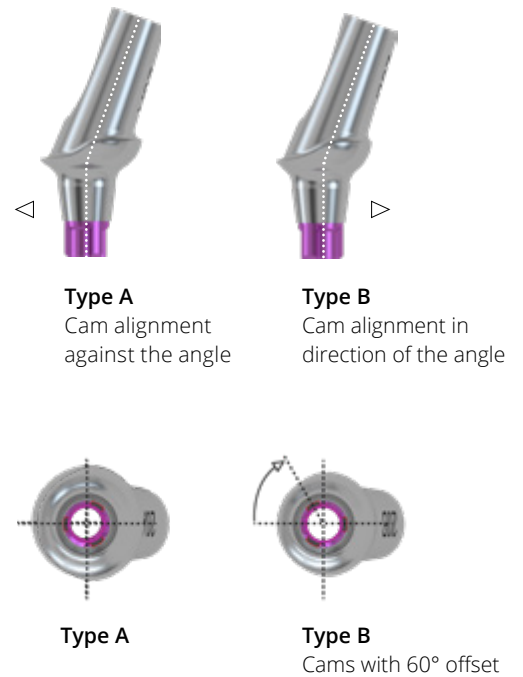

## CONELOG® Disconnecter for CONELOG® Abutments

The CONELOG® Implant-abutment connection is characterized by a self-locking taper. A special CONELOG® Disconnecter is available for the easy removal of CONELOG® Abutments from CONELOG® Implants or lab analogs. First, the CONELOG® Abutment screw or the lab screw is removed and the disconnecter is screwed into the screw canal until the abutment releases from the internal taper of the CONELOG® Implant or lab analog.



## CONELOG® Universal and telescope abutments

CONELOG® Universal and telescope abutments can be used for individually fabricated cementable crown and bridge restorations and for double crown restorations. The abutments are made of titanium alloy and can be custom trimmed.


## CONELOG® Titanium bases CAD/CAM

CONELOG® Titanium bases CAD/CAM act as a bonding basis for customized, implant-supported dental restorations made of suitable materials. Reconstructions are fabricated with the aid of CAD/CAM techniques. CONELOG® Titanium bases CAD/CAM are available in crown and bridge versions, each with gingival heights of 1.0 and 2.0 mm.



## CONELOG® Ball, Locator® and straight bar abutments

Ball, Locator® and straight bar abutments are available for the CONELOG® Implant System. These differ from the abutments in the apical area through different connection designs. Ball, Locator® and straight bar abutments are manufactured as single units with a thread in the apical region which engages with the inner thread of the CONELOG® Implant. These abutments are screwed into the CONELOG® Implant using the corresponding insertion tools.

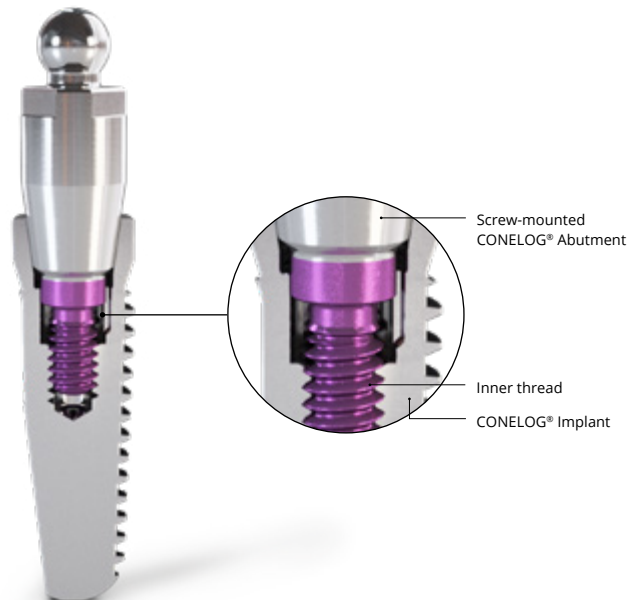


**Example: CONELOG® Ball abutment (Ø 4.3 m)  
in a CONELOG® SCREW-LINE Implant**

## COMFOUR® System

Occlusal screw-mounted restorations are state-of-the-art. With the COMFOUR® System, edentulous patients are given the option of immediate, comfortable, and fixed dentures based on four or six implants as a rule, with a huge gain in their quality of life. Clinicians too can look forward to considerably greater comfort and freedom. COMFOUR® provides several treatment options. In addition to occlusal screw-mounted crowns and bridges for immediate and delayed restorations, the multi-option system also permits bar restorations on straight and angled bar abutments. COMFOUR® offers a range of options to master the challenges faced in routine practice with greater ease and in less time.

Next to its versatility, the COMFOUR® Prosthetic System is particularly impressive thanks to its slim design.

All components are of a delicate and low design, which simplifies prosthetic restorations considerably for dentists and dental technicians. In addition, a number of technical highlights ensure that COMFOUR® is not simply just a name but also a program—for users and patients alike.

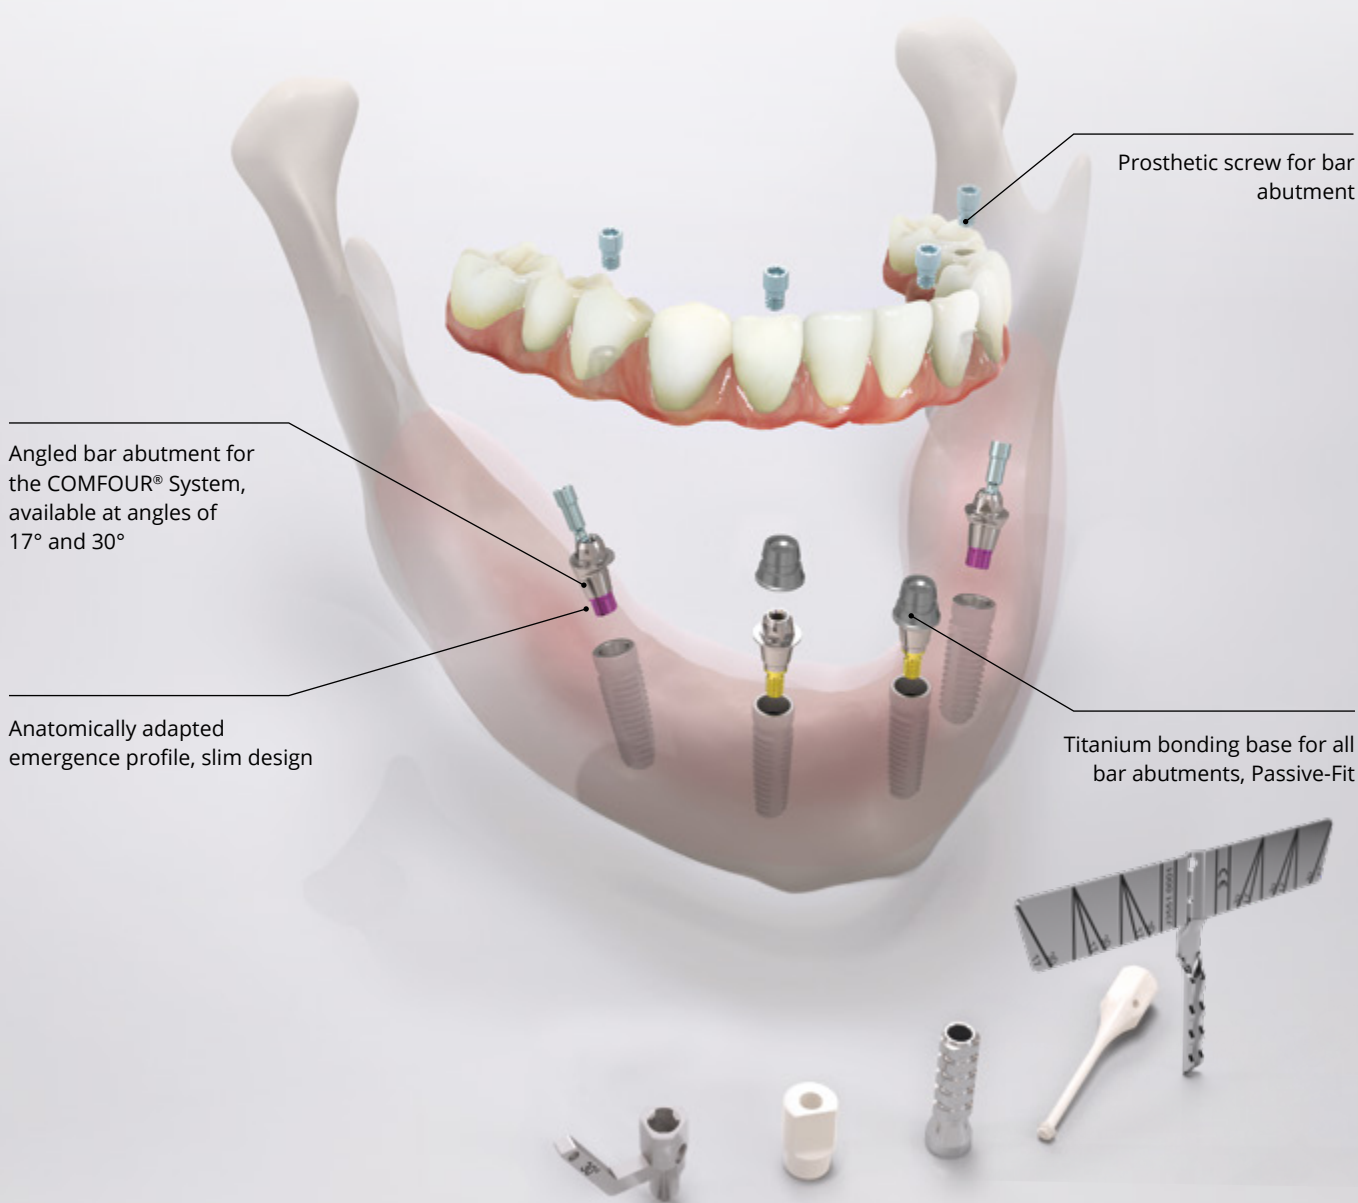

COMFOUR® offers a large selection of options to manage the requirements of your practice.

## CAD/CAM services

Individually CAD/CAM fabricated prosthetics, healing caps and impression posts, scanning and design services, 3D implant planning, printed drilling templates and jaw models are available from Camlog through our DEDICAM® Service Division.

Personal support with the accustomed competence of our employees as well as processes optimized right down to the finest detail ensure a high degree of certainty of results with the greatest possible individual freedom.
























Extensive libraries for the open CAD systems from 3Shape, exocad and Dental Wings are available for implant-supported restorations.



## DEDICAM® DIGITAL CONCEPTS

Discover your options and start your digital future with DEDICAM®.  
DEDICAM® Services are not available in all countries. Please ask your local Camlog representative for details.


## Explanation of symbols

	CE marking
	CE marking with number of the Notified Body
	Consult Instructions for Use
	Caution, observe the warning notices
	Medical Device
	Article number
	Lot number
	Serial number
	Sterilized using irradiation
	Single sterile barrier system with protective packaging outside
	Single sterile barrier
	Non-sterile
	Date of manufacture
	Use-by date
	Do not resterilize
	Do not reuse
	Do not use if package is damaged
	Protect against sunlight
	Temperature limit
	Manufacturer
	MR Conditional
	Contains hazardous substances
	Caution: US Federal law restricts this device to sale by or on the order of a dentist or physician.

## Explanation of abbreviations

$\emptyset$	Diameter
A $\emptyset$	Apical diameter
G $\emptyset$	Gingival diameter
PP $\emptyset$	Prosthetic platform diameter
L	Length
GH	Gingival height
PEEK	Poly ether ether ketone
POM	Polyoxymethylene
PPSU	Polyphenylsulfone

## Color coding of the surgical and prosthetic CONELOG® Products

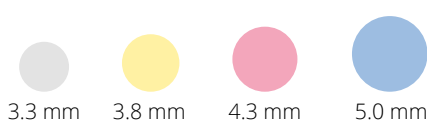

## General safety instructions and warnings

- The descriptions in this product catalog are not sufficient to allow immediate use of the CONELOG® Implant System.
- Instruction by a surgeon experienced in using the CONELOG® Implant System is strongly recommended. CONELOG® Products may only be applied by dentists, physicians, surgeons and dental technicians trained on the system. Appropriate courses and training sessions are offered by Camlog.
- Methodical errors made during the treatment can result in loss of the implant and significant loss of the peri-implant bone.
- The images in this document are for reference purposes only and may differ from the actual product.

## Packaging of PROGRESSIVE-LINE Implants

### Secondary packaging


Sealed, folding box with color-coded product label

### Inner implant packaging (primary packaging)

Sealed, color-coded



Example of product label for outer packaging of the implant

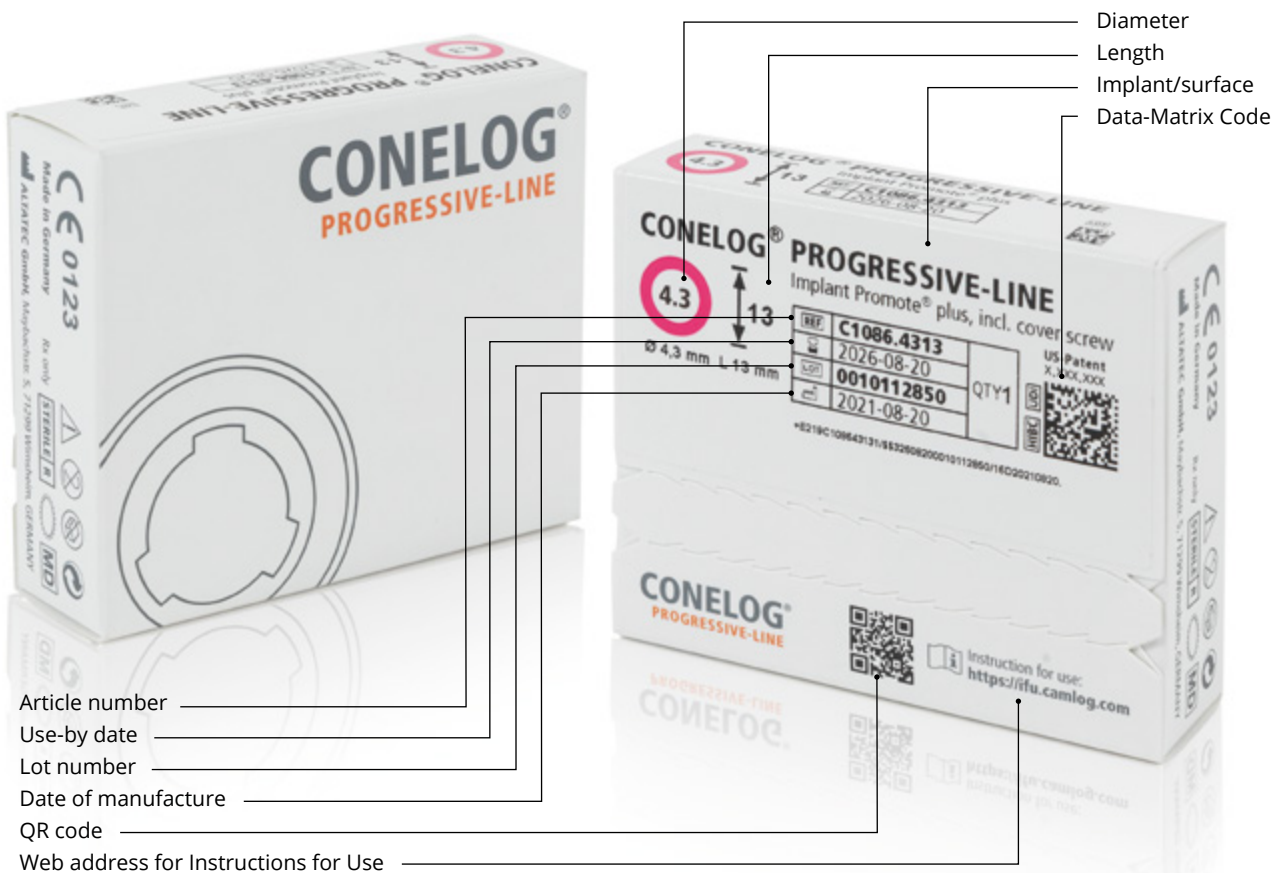



## Packaging of SCREW-LINE Implants

### Secondary packaging

Sealed, folding box with color-coded product label

### Inner implant packaging (primary packaging)

Sealed, color-coded



Example of product label for outer packaging of the implant



Packaging units: unless described otherwise, each pack contains one product.



New

**Direct part marking – better identification and traceability**






In future, all Camlog instruments will feature a label with the lot number and/or UDI code in addition to the article number. This makes it easier for the entire practice team to identify and assign the products. The product images contained in the catalog do not yet always reflect this specification.

# Surgery





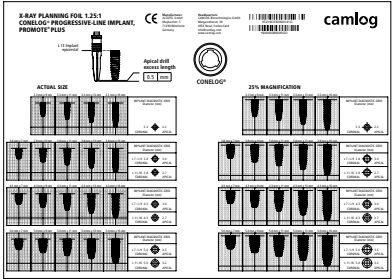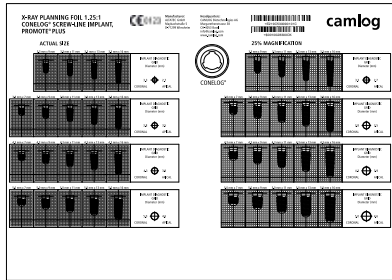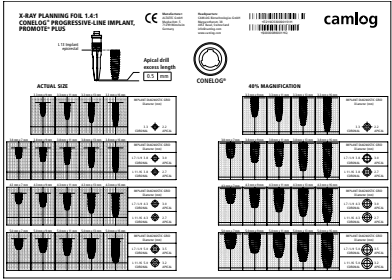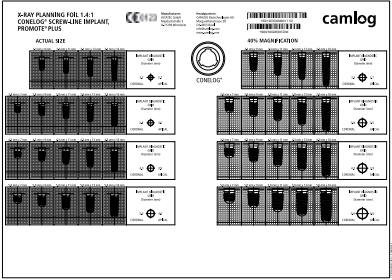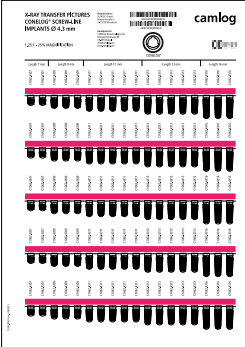

# Planning

## X-Ray Planning foils and X-Ray Transfer pictures

	Article	Art. No.	Ø
	<p>X-Ray Planning foil 1.25:1  <b>CONELOG® PROGRESSIVE-LINE Implants</b>            Magnification 25 %</p>	C5300.9014	-
	<p>X-Ray Planning foil 1.25:1  <b>CONELOG® SCREW-LINE Implants</b>            Magnification 25 %</p>	C5300.9010	-
	<p>X-Ray Planning foil 1.4:1  <b>CONELOG® PROGRESSIVE-LINE Implants</b>            Magnification 40 %</p>	C5300.9015	-
	<p>X-Ray Planning foil 1.4:1  <b>CONELOG® SCREW-LINE Implants</b>            Magnification 40 %</p>	C5300.9011	-
	<p>X-Ray Transfer pictures 1.25:1  <b>CONELOG® SCREW-LINE Implants</b>            Planning foils,            self-adhesive            Magnification 25 %</p>	C5300.9080	3.3 mm
		C5300.9081	3.8 mm
		C5300.9082	4.3 mm
		C5300.9083	5.0 mm


# CT-Planning

## for 3D X-ray and drilling templates

	Article	Art. No.	L
	<b>Tubing for CT planning</b> for drill Ø 2.0 mm*, corrugated tubing (10 units) internal diameter 2.1 mm external diameter 2.5 mm  <b>Material</b> Titanium alloy	A2002.2000	4.0 mm 10.0 mm
	<b>Tubing for CT planning</b> for drill Ø 2.2 mm, corrugated tubing (10 units) internal diameter 2.3 mm external diameter 2.7 mm  <b>Material</b> Titanium alloy	A2222.2200	4.0 mm 10.0 mm
	<b>Drill for placement of corrugated CT-tubes (for A2002.2000)</b> Ø 2.6 mm  <b>Material</b> Stainless steel	A2050.2600	-
	<b>Drill for placement of corrugated CT-tubes (for A2222.2200)</b> Ø 2.8 mm  <b>Material</b> Stainless steel	A2050.2800	-


\* for pilot drills J5051.2003 and pilot drills SCREW-LINE J5051.2000

# PROGRESSIVE-LINE

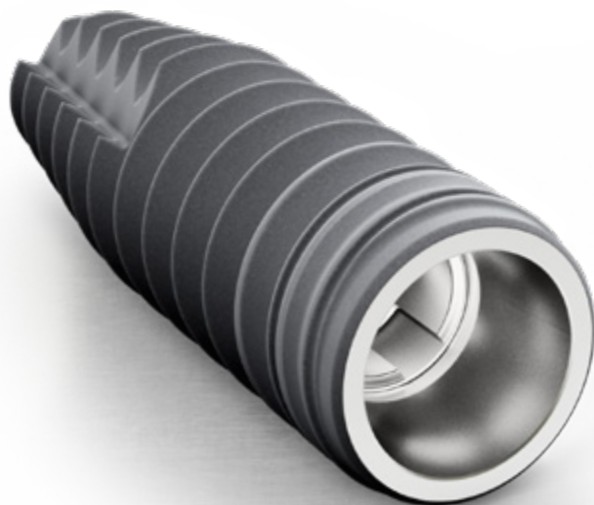


# PROGRESSIVE-LINE

## Implants with snap-in insertion posts

	Article	Art. No.	Ø	L	A Ø	
	<b>CONELOG® PROGRESSIVE-LINE Implant, Promote® plus</b> incl. snap-in insertion post and cover screw, sterile  <b>Material</b> Titanium Grade 4	C1086.3309	3.3 mm	9 mm	2.2 mm	
		C1086.3311		11 mm		
		C1086.3313		13 mm		
		C1086.3316		16 mm		
		C1086.3807	3.8 mm	7 mm	3.0 mm	
		C1086.3809		9 mm		
		C1086.3811		11 mm		
		C1086.3813		13 mm		
		C1086.3816	16 mm	2.7 mm		
		C1086.4307	4.3 mm		7 mm	3.0 mm
		C1086.4309			9 mm	
		C1086.4311			11 mm	
		C1086.4313		13 mm		
		C1086.4316	16 mm	2.7 mm		
		C1086.5007	5.0 mm		7 mm	3.5 mm
		C1086.5009			9 mm	
		C1086.5011			11 mm	
		C1086.5013		13 mm		
C1086.5016	16 mm	3.2 mm				

Surgery


## Implants with screw-mounted insertion posts

	Article	Art. No.	Ø	L	A Ø	
	<b>CONELOG® PROGRESSIVE-LINE Implant, Promote® plus</b> incl. screw-mounted insertion post and cover screw, sterile  <b>Material</b> Titanium Grade 4	C1085.3309	3.3 mm	9 mm	2.2 mm	
		C1085.3311		11 mm		
		C1085.3313		13 mm		
		C1085.3316		16 mm		
		C1085.3807	3.8 mm	7 mm	3.0 mm	
		C1085.3809		9 mm		
		C1085.3811		11 mm		
		C1085.3813		13 mm		
		C1085.3816	16 mm	2.7 mm		
		C1085.4307	4.3 mm		7 mm	3.0 mm
		C1085.4309			9 mm	
		C1085.4311			11 mm	
		C1085.4313		13 mm		
		C1085.4316	16 mm	2.7 mm		
		C1085.5007	5.0 mm		7 mm	3.5 mm
		C1085.5009			9 mm	
		C1085.5011			11 mm	
		C1085.5013		13 mm		
C1085.5016	16 mm	3.2 mm				

**Note**  
 Implants with the screw-mounted insertion post (Art. No. C1085.xxxx) are to be used for template-guided implant insertion with the PROGRESSIVE-LINE Guide System.

# PROGRESSIVE-LINE

## Surgery Set CAMLOG®/CONELOG®

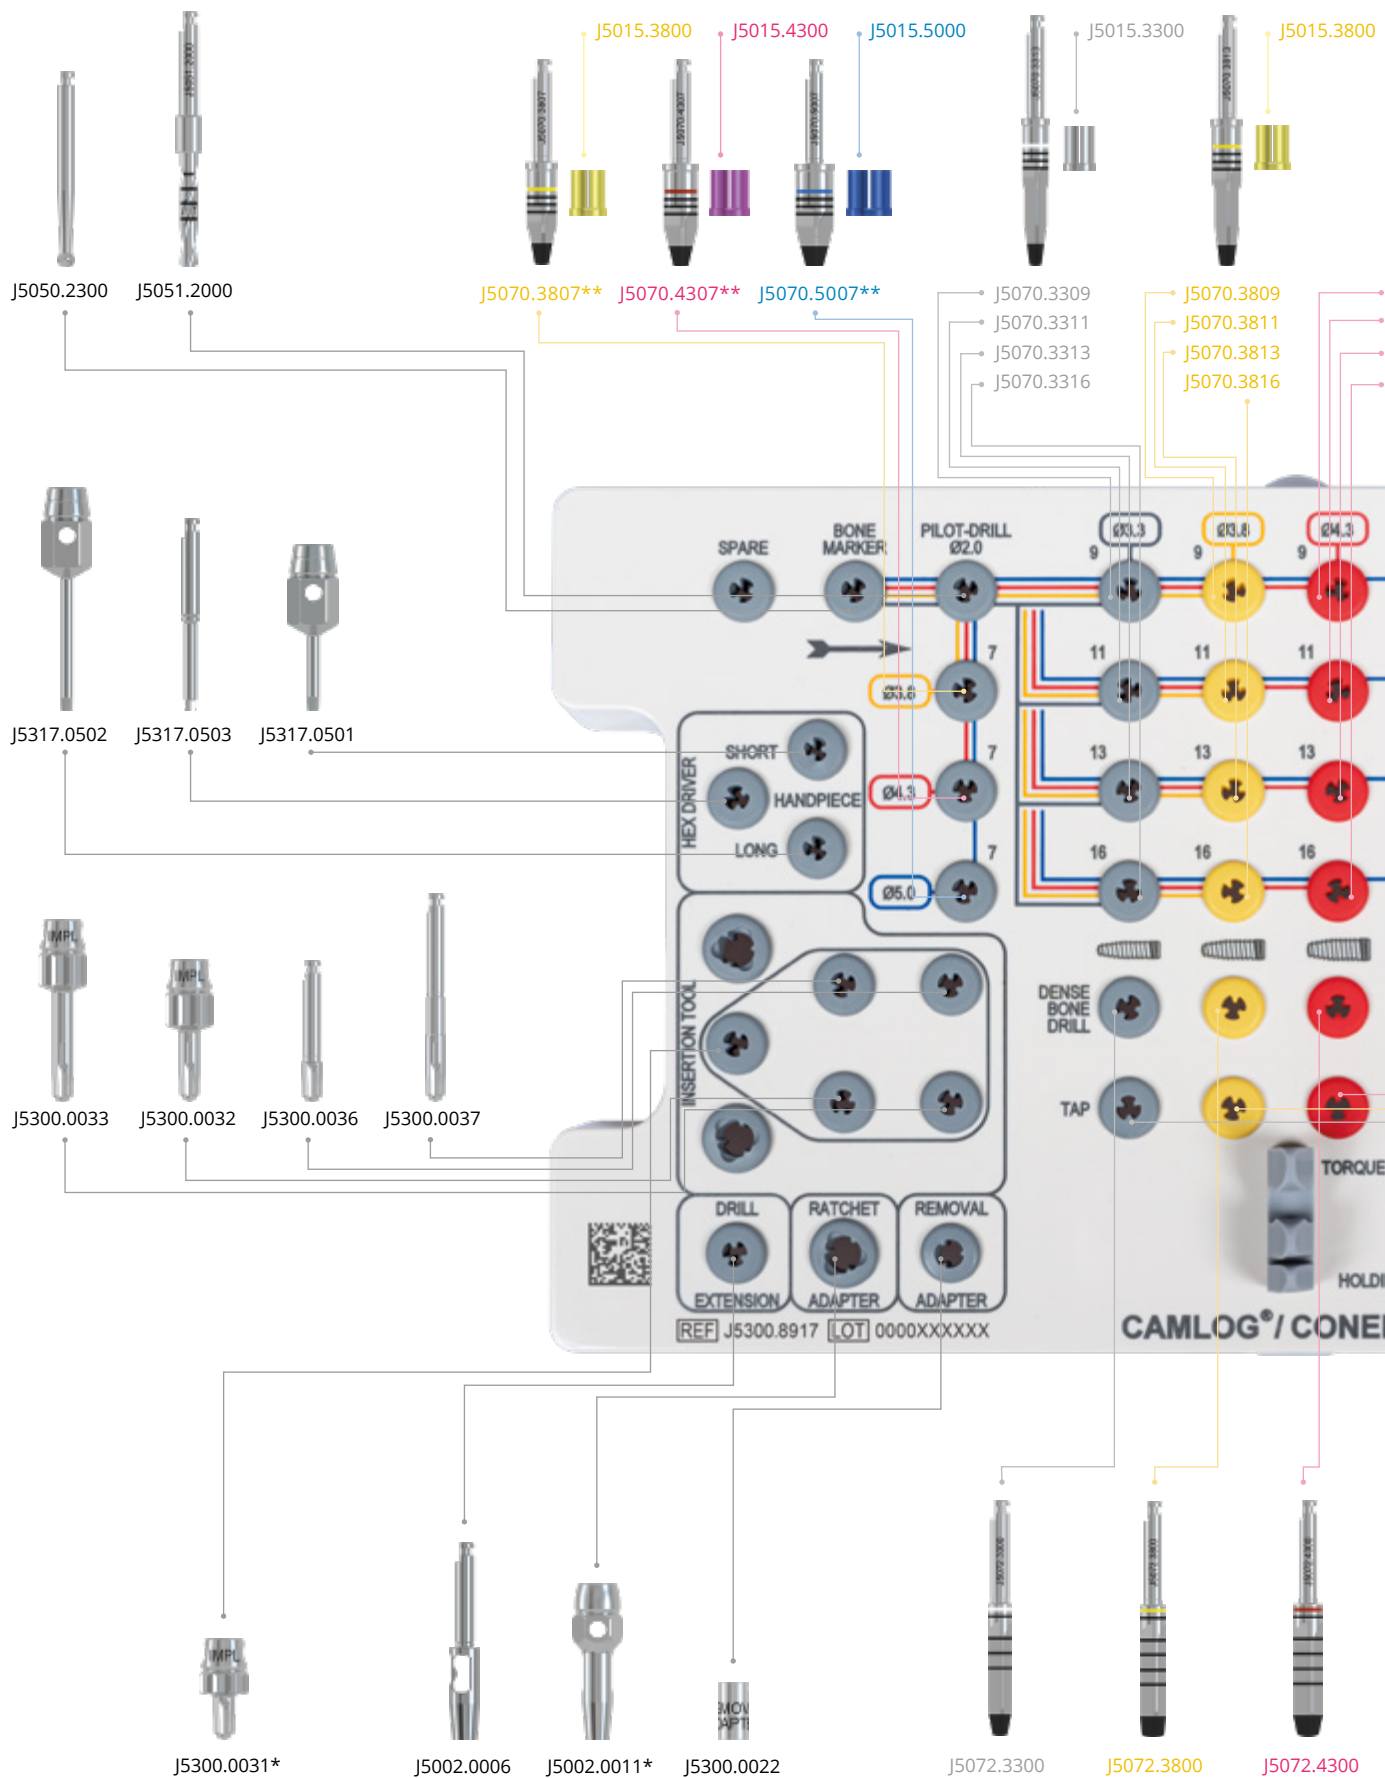

\* These articles are not included in the surgery set and must be ordered separately.





**Note**

- The drills are arranged and sorted in the set according to the treatment sequence.
- Colored lines indicate the exact drilling sequence.

- J5070.4309
- J5070.4311
- J5070.4313
- J5070.4316
- J5070.5009
- J5070.5011
- J5070.5013
- J5070.5016



J5300.2000



J5015.0013



J5015.0011



J5015.0009




J5015.0007



J5320.1030


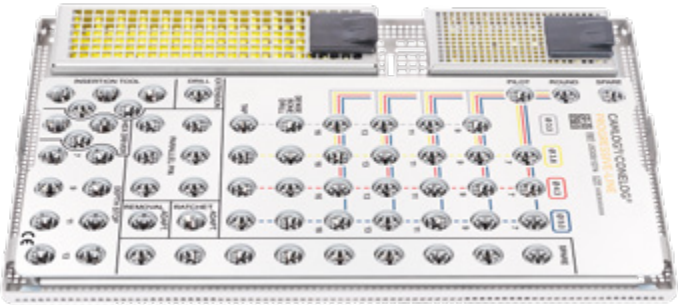
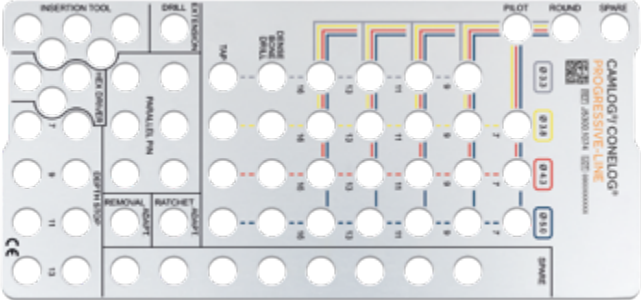


J5302.0010

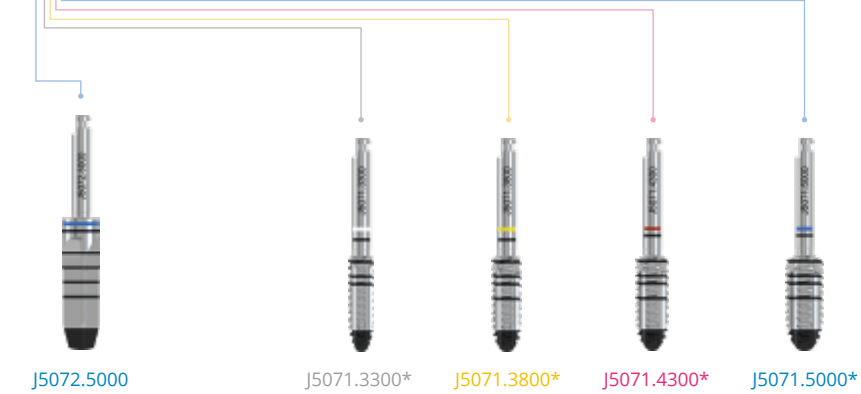






# PROGRESSIVE-LINE

## Surgery set and wash tray

	Article	Art. No.
 <p>The image shows a white plastic surgery set tray. It contains various surgical instruments organized by color-coded handles: blue, yellow, red, and black. There are also several blue-handled instruments. A torque wrench and a universal holding key are also visible. The tray has a handle on the right side and the text 'CAMLOG® CONELOG® PROGRESSIVE-LINE' printed on the bottom.</p>	<p><b>Surgery Set</b>  <b>CAMLOG®/CONELOG®</b>  <b>PROGRESSIVE-LINE</b>            contains all necessary color-code ordered surgical instruments, incl. torque wrench and universal holding key (taps are not included)</p>	<p>J5300.0065</p>
 <p>The image shows a stainless steel surgery wash tray. It has a grid of circular holes for instruments. The tray is labeled with 'CAMLOG®/CONELOG® PROGRESSIVE-LINE' and 'incl. pattern, without content'. There are also some yellow and black components on the tray.</p>	<p><b>Surgery wash tray</b>  <b>CAMLOG®/CONELOG®</b>  <b>PROGRESSIVE-LINE</b>            incl. pattern, without content</p>	<p>J5300.8970</p>
 <p>The image shows a stainless steel pattern for the surgery wash tray. It has a grid of circular holes and is labeled with 'CAMLOG®/CONELOG® PROGRESSIVE-LINE' and 'Material Stainless steel'. The pattern is used to create the wash tray.</p>	<p><b>Pattern for surgery wash tray</b>  <b>CAMLOG®/CONELOG®</b>  <b>PROGRESSIVE-LINE</b>  <b>Material</b>            Stainless steel</p>	<p>J5300.1074</p>

Preparation of the implant bed for CAMLOG® PROGRESSIVE-LINE Implants and for CONELOG® PROGRESSIVE-LINE Implants is performed with identical instruments.

## Surgical instruments

	Article	Art. No.	Ø	L
	<b>Form drills</b> <b>PROGRESSIVE-LINE</b> resterilizable  <b>Material</b> Stainless steel	J5070.3309	3.3 mm	9 mm
		J5070.3311		11 mm
		J5070.3313		13 mm
		J5070.3316		16 mm
		J5070.3807	3.8 mm	7 mm
		J5070.3809		9 mm
		J5070.3811		11 mm
		J5070.3813		13 mm
		J5070.3816	16 mm	
		J5070.4307	4.3 mm	7 mm
		J5070.4309		9 mm
		J5070.4311		11 mm
		J5070.4313		13 mm
		J5070.4316	16 mm	
		J5070.5007	5.0 mm	7 mm
		J5070.5009		9 mm
J5070.5011	11 mm			
J5070.5013	13 mm			
J5070.5016	16 mm			
	<b>Depth stop, for form drills</b> <b>PROGRESSIVE-LINE and SCREW-LINE</b> resterilizable  <b>Material</b> Titanium alloy	J5015.3300	3.3 mm	-
		J5015.3800	3.8 mm	
		J5015.4300	4.3 mm	
		J5015.5000	5.0 mm	
	<b>Dense bone drill</b> <b>PROGRESSIVE-LINE</b> resterilizable  <b>Material</b> Stainless steel	J5072.3300	3.3 mm	-
		J5072.3800	3.8 mm	
		J5072.4300	4.3 mm	
		J5072.5000	5.0 mm	
	<b>Tap</b> <b>PROGRESSIVE-LINE</b> resterilizable  <b>Material</b> Stainless steel	J5071.3300	3.3 mm	-
		J5071.3800	3.8 mm	
		J5071.4300	4.3 mm	
		J5071.5000	5.0 mm	
	<b>Paralleling pin</b> <b>PROGRESSIVE-LINE</b> with depth marks (for pilot drilling Ø 2.0 mm)  <b>Material</b> Titanium alloy	J5300.2000	-	-


# PROGRESSIVE-LINE Guide System






# PROGRESSIVE-LINE Guide System



Surgery tray CAMLOG®/CONELOG®

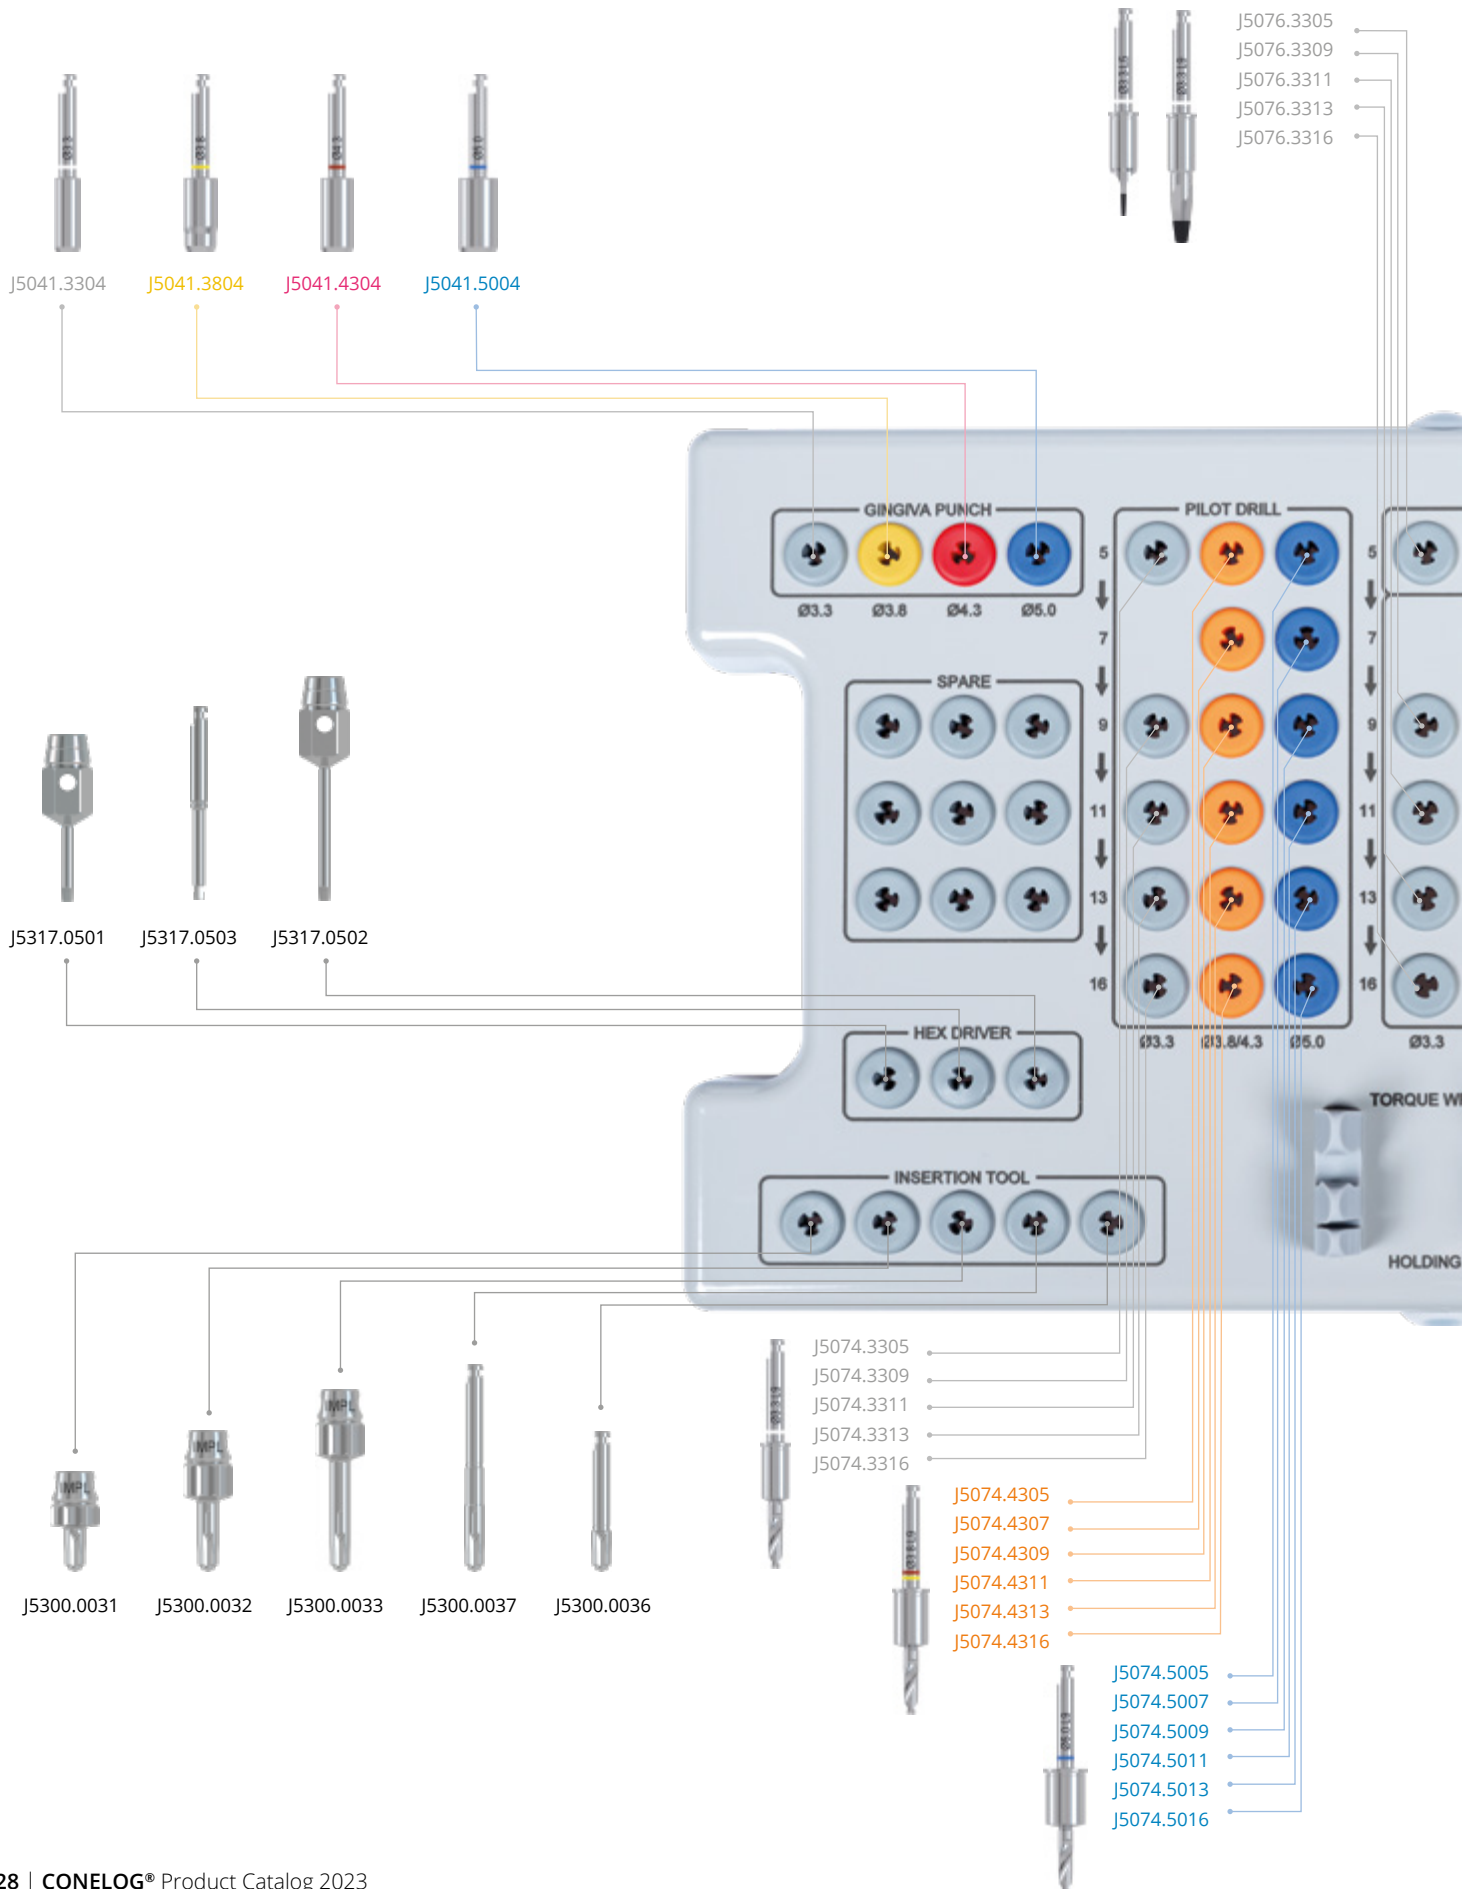

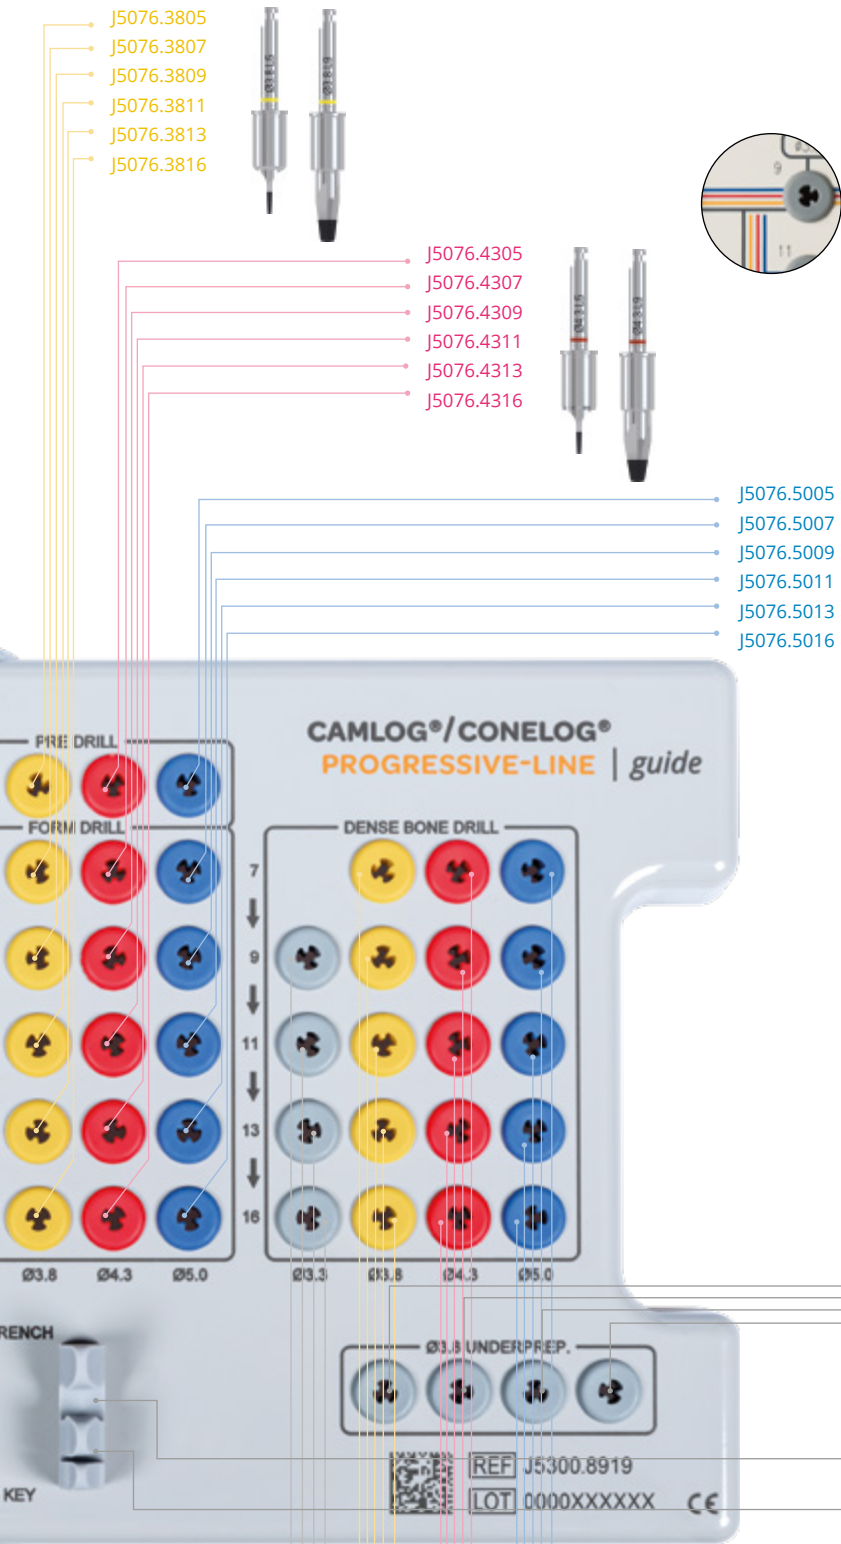

**Note**

- The drills are arranged and sorted in the set according to the treatment sequence.
- Colored lines indicate the exact drilling sequence.

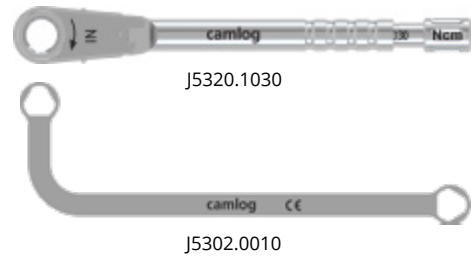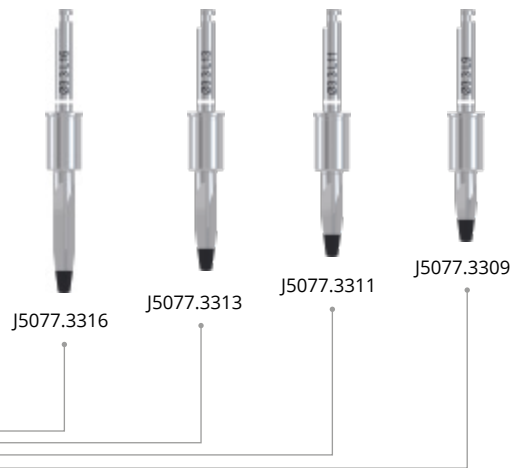

- J5078.3309**  
**J5078.3311**  
**J5078.3313**  
**J5078.3316**
- J5078.3807**  
**J5078.3809**  
**J5078.3811**  
**J5078.3813**  
**J5078.3816**
- J5078.4307**  
**J5078.4309**  
**J5078.4311**  
**J5078.4313**  
**J5078.4316**
- J5078.5007**  
**J5078.5009**  
**J5078.5011**  
**J5078.5013**  
**J5078.5016**



# PROGRESSIVE-LINE Guide System

## Surgery and wash tray





	Article	Art. No.
	<p>Guide System surgery tray CAMLOG®/CONELOG® PROGRESSIVE-LINE without content</p>	<p>J5300.8919</p>
	<p>Guide System surgery wash tray CAMLOG®/CONELOG® PROGRESSIVE-LINE incl. pattern, without content</p> <p><b>Material</b> Stainless steel</p>	<p>J5300.8971</p>
	<p>Guide System pattern for surgery wash tray CAMLOG®/CONELOG® PROGRESSIVE-LINE</p> <p><b>Material</b> Stainless steel</p>	<p>J5300.1072</p>

**Note**

Implants with the screw-mounted insertion post (Art. No. C1085.xxxx) are to be used for template-guided implant insertion with the PROGRESSIVE-LINE Guide System.






## Surgical instruments

	Article	Art. No.	Ø	L	
	<b>Guide System gingiva punch</b> <b>PROGRESSIVE-LINE</b> resterilizable  <b>Material</b> Stainless steel	J5041.3304	3.3 mm	-	
		J5041.3804	3.8 mm		
		J5041.4304	4.3 mm		
		J5041.5004	5.0 mm		
	<b>Guide System pilot drills</b> <b>PROGRESSIVE-LINE</b> resterilizable  <b>Material</b> Stainless steel	J5074.3305	3.3 mm	5 mm	
		J5074.3309		9 mm	
		J5074.3311		11 mm	
		J5074.3313		13 mm	
		J5074.3316		16 mm	
		J5074.4305	3.8 mm	4.3 mm	5 mm
		J5074.4307			7 mm
		J5074.4309	5.0 mm		9 mm
		J5074.4311			11 mm
		J5074.4313			13 mm
		J5074.4316			16 mm
		J5074.5005	5.0 mm		5 mm
		J5074.5007			7 mm
		J5074.5009			9 mm
		J5074.5011			11 mm
		J5074.5013			13 mm
J5074.5016	16 mm				
	<b>Guide System pre-drill</b> <b>PROGRESSIVE-LINE</b> resterilizable  <b>Material</b> Stainless steel	J5076.3305	3.3 mm	5 mm	
		J5076.3805	3.8 mm		
		J5076.4305	4.3 mm		
		J5076.5005	5.0 mm		
	<b>Guide System form drills</b> <b>PROGRESSIVE-LINE</b> resterilizable  <b>Material</b> Stainless steel	J5076.3309	3.3 mm	9 mm	
		J5076.3311		11 mm	
		J5076.3313		13 mm	
		J5076.3316		16 mm	
		J5076.3807	3.8 mm		7 mm
		J5076.3809			9 mm
		J5076.3811			11 mm
		J5076.3813			13 mm
		J5076.3816			16 mm
		J5076.4307	4.3 mm		7 mm
		J5076.4309			9 mm
		J5076.4311			11 mm
		J5076.4313			13 mm
		J5076.4316	5.0 mm		16 mm
		J5076.5007			7 mm
		J5076.5009			9 mm
		J5076.5011			11 mm
		J5076.5013			13 mm
J5076.5016	16 mm				

# PROGRESSIVE-LINE Guide System

## Surgical instruments

	Article	Art. No.	Ø	L
	<b>Guide System dense bone drill PROGRESSIVE-LINE</b> resterilizable  <b>Material</b> Stainless steel	J5078.3309	3.3 mm	9 mm
		J5078.3311		11 mm
		J5078.3313		13 mm
		J5078.3316		16 mm
		J5078.3807	3.8 mm	7 mm
		J5078.3809		9 mm
		J5078.3811		11 mm
		J5078.3813		13 mm
		J5078.3816	16 mm	
		J5078.4307	4.3 mm	7 mm
		J5078.4309		9 mm
		J5078.4311		11 mm
		J5078.4313		13 mm
		J5078.4316	16 mm	
		J5078.5007	5.0 mm	7 mm
		J5078.5009		9 mm
		J5078.5011		11 mm
J5078.5013	13 mm			
J5078.5016	16 mm			
	<b>Guide System form drill for Ø 3.8 mm underpreparation PROGRESSIVE-LINE</b> resterilizable  <b>Material</b> Stainless steel	J5077.3309	3.3 mm	9 mm
		J5077.3311		11 mm
		J5077.3313		13 mm
		J5077.3316		16 mm
	<b>Guide System guiding sleeve PROGRESSIVE-LINE</b> (2 units)  <b>Material</b> Titanium alloy	J3754.3301*	3.3 mm	-
		J3754.3801*	3.8 mm	
		J3754.4301*	4.3 mm	
		J3754.5001*	5.0 mm	


\* The sleeves are not compatible with the SCREW-LINE Guide System.

# PROGRESSIVE-LINE Flex



# PROGRESSIVE-LINE Flex

## Surgery Set CAMLOG®/CONELOG®

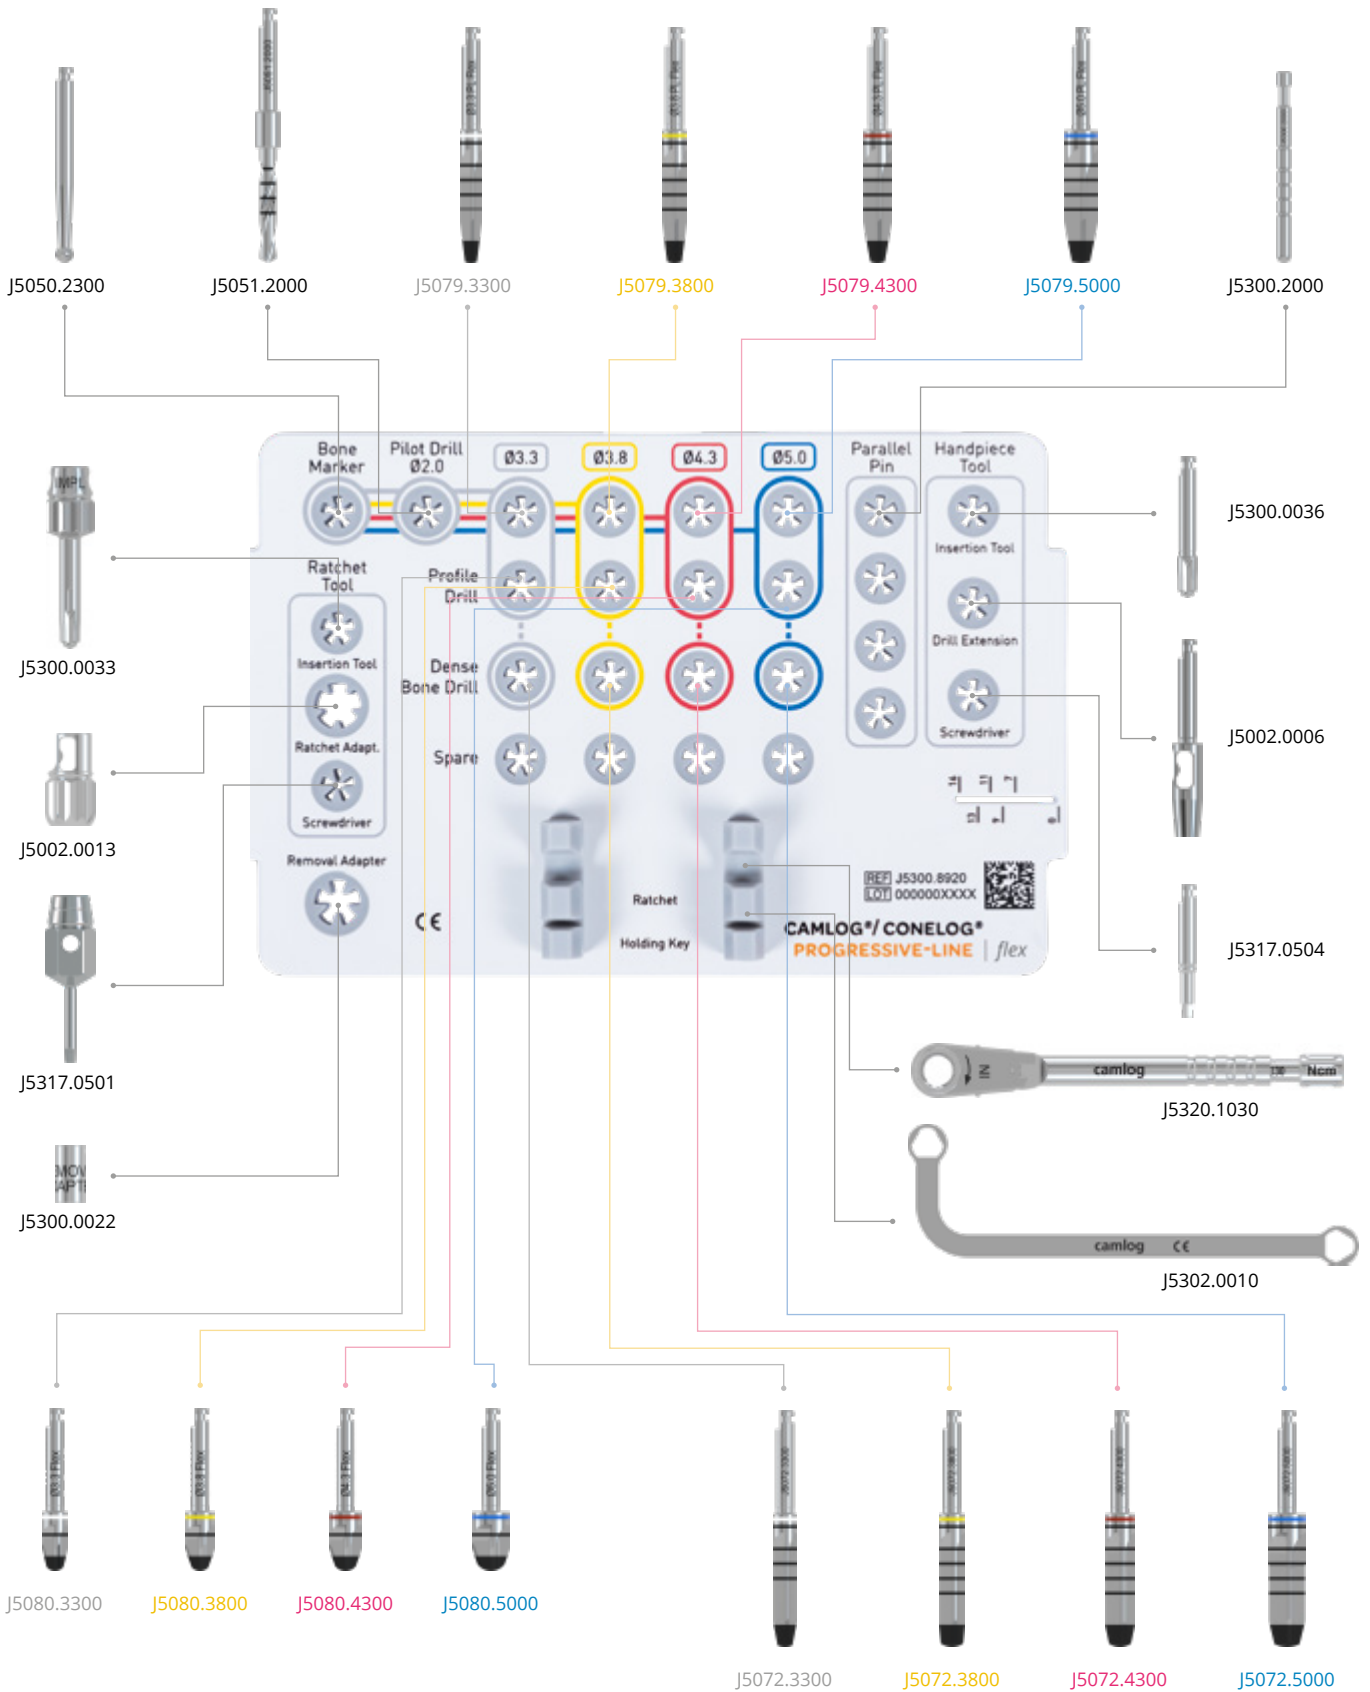

### Note






- The drills are arranged and sorted in the set according to the treatment sequence.
- Colored lines indicate the exact drilling sequence.

## Surgery Set



	Article	Art. No.
	<p><b>Surgery Set</b>  <b>CAMLOG®/CONELOG®</b>  <b>PROGRESSIVE-LINE Flex</b>            contains all necessary            color-code ordered surgical            instruments, incl. torque            wrench and universal holding key</p>	<p>J5300.0071</p>

# PROGRESSIVE-LINE Flex

## Surgical instruments


	Article	Art. No.	Ø	L
	<b>Drill</b> <b>PROGRESSIVE-LINE Flex</b> resterilizable  <b>Material</b> Stainless steel	J5079.3300	3.3 mm	-
		J5079.3800	3.8 mm	
		J5079.4300	4.3 mm	
		J5079.5000	5.0 mm	
	<b>Profile drill</b> <b>PROGRESSIVE-LINE Flex</b> resterilizable  <b>Material</b> Stainless steel	J5080.3300	3.3 mm	-
		J5080.3800	3.8 mm	
		J5080.4300	4.3 mm	
		J5080.5000	5.0 mm	
	<b>Dense bone drill</b> <b>PROGRESSIVE-LINE</b> resterilizable  <b>Material</b> Stainless steel	J5072.3300	3.3 mm	-
		J5072.3800	3.8 mm	
		J5072.4300	4.3 mm	
		J5072.5000	5.0 mm	
	<b>Tap</b> <b>PROGRESSIVE-LINE</b> resterilizable  <b>Material</b> Stainless steel	J5071.3300	3.3 mm	-
		J5071.3800	3.8 mm	
		J5071.4300	4.3 mm	
		J5071.5000	5.0 mm	
	<b>Wrench adapter</b>  <b>Material</b> Stainless steel	J5002.0013	-	11 mm

# SCREW-LINE

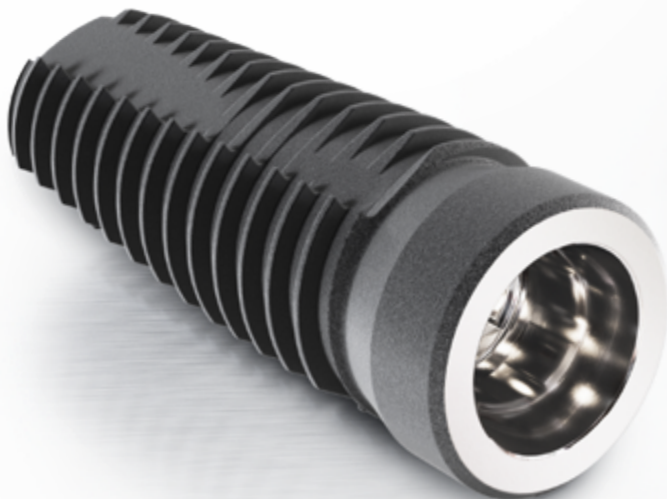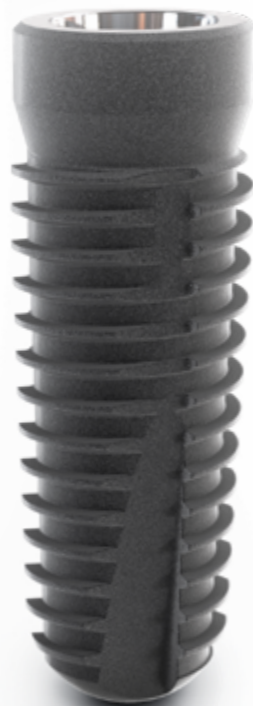

# SCREW-LINE

## Implants with snap-in insertion posts


	Article	Art. No.	Ø	L	A Ø
	<b>CONELOG® SCREW-LINE Implant, Promote® plus</b> incl. snap-in insertion post and cover screw, sterile  <b>Material</b> Titanium Grade 4	C1066.3309	3.3 mm	9 mm	2.7 mm
		C1066.3311		11 mm	
		C1066.3313		13 mm	
		C1066.3316		16 mm	
		C1066.3807	3.8 mm	7 mm	3.5 mm
		C1066.3809		9 mm	
		C1066.3811		11 mm	
		C1066.3813		13 mm	
		C1066.3816	16 mm	3.9 mm	
		C1066.4307	7 mm		
		C1066.4309	9 mm		
		C1066.4311	11 mm		
		C1066.4313	13 mm	4.6 mm	
		C1066.4316	16 mm		
		C1066.5007	7 mm		
		C1066.5009	9 mm		
		C1066.5011	11 mm	5.0 mm	
		C1066.5013	13 mm		
		C1066.5016	16 mm		

### Note

CONELOG® SCREW-LINE implants, Promote® plus, with Art. No. C1066.xxxx and C1065-xxxx can be used exclusively with the insertion tools (Art. No. J5300.0031, J5300.0032, J5300.0033, J5300.0034 or J5300.0035, J5300.0036 and J5300.0037).



## Implants with screw-mounted insertion posts

	Article	Art. No.	Ø	L	A Ø
	<b>CONELOG® SCREW-LINE Implant, Promote® plus</b> incl. screw-mounted insertion post and cover screw, sterile  <b>Material</b> Titanium Grade 4	C1065.3309	3.3 mm	9 mm	2.7 mm
		C1065.3311		11 mm	
		C1065.3313		13 mm	
		C1065.3316		16 mm	
		C1065.3807	3.8 mm	7 mm	3.5 mm
		C1065.3809		9 mm	
		C1065.3811		11 mm	
		C1065.3813		13 mm	
		C1065.3816	16 mm	3.9 mm	
		C1065.4307	7 mm		
		C1065.4309	9 mm		
		C1065.4311	11 mm		
		C1065.4313	13 mm	4.6 mm	
		C1065.4316	16 mm		
		C1065.5007	7 mm		
		C1065.5009	9 mm		
		C1065.5011	5.0 mm	11 mm	4.6 mm
		C1065.5013		13 mm	
		C1065.5016		16 mm	

**Note**


Implants with the screw-mounted insertion post (Art. No. C10655.xxxx) are to be used for template-guided implant insertion with the SCREW-LINE Guide System.

**Note**

CONELOG® SCREW-LINE implants, Promote® plus, with Art. No. C1066.xxxx and C1065-xxxx can be used exclusively with the insertion tools (Art. No. J5300.0031, J5300.0032, J5300.0033, J5300.0034 or J5300.0035, J5300.0036 and J5300.0037).

# SCREW-LINE

## Surgery Set CAMLOG®/CONELOG®

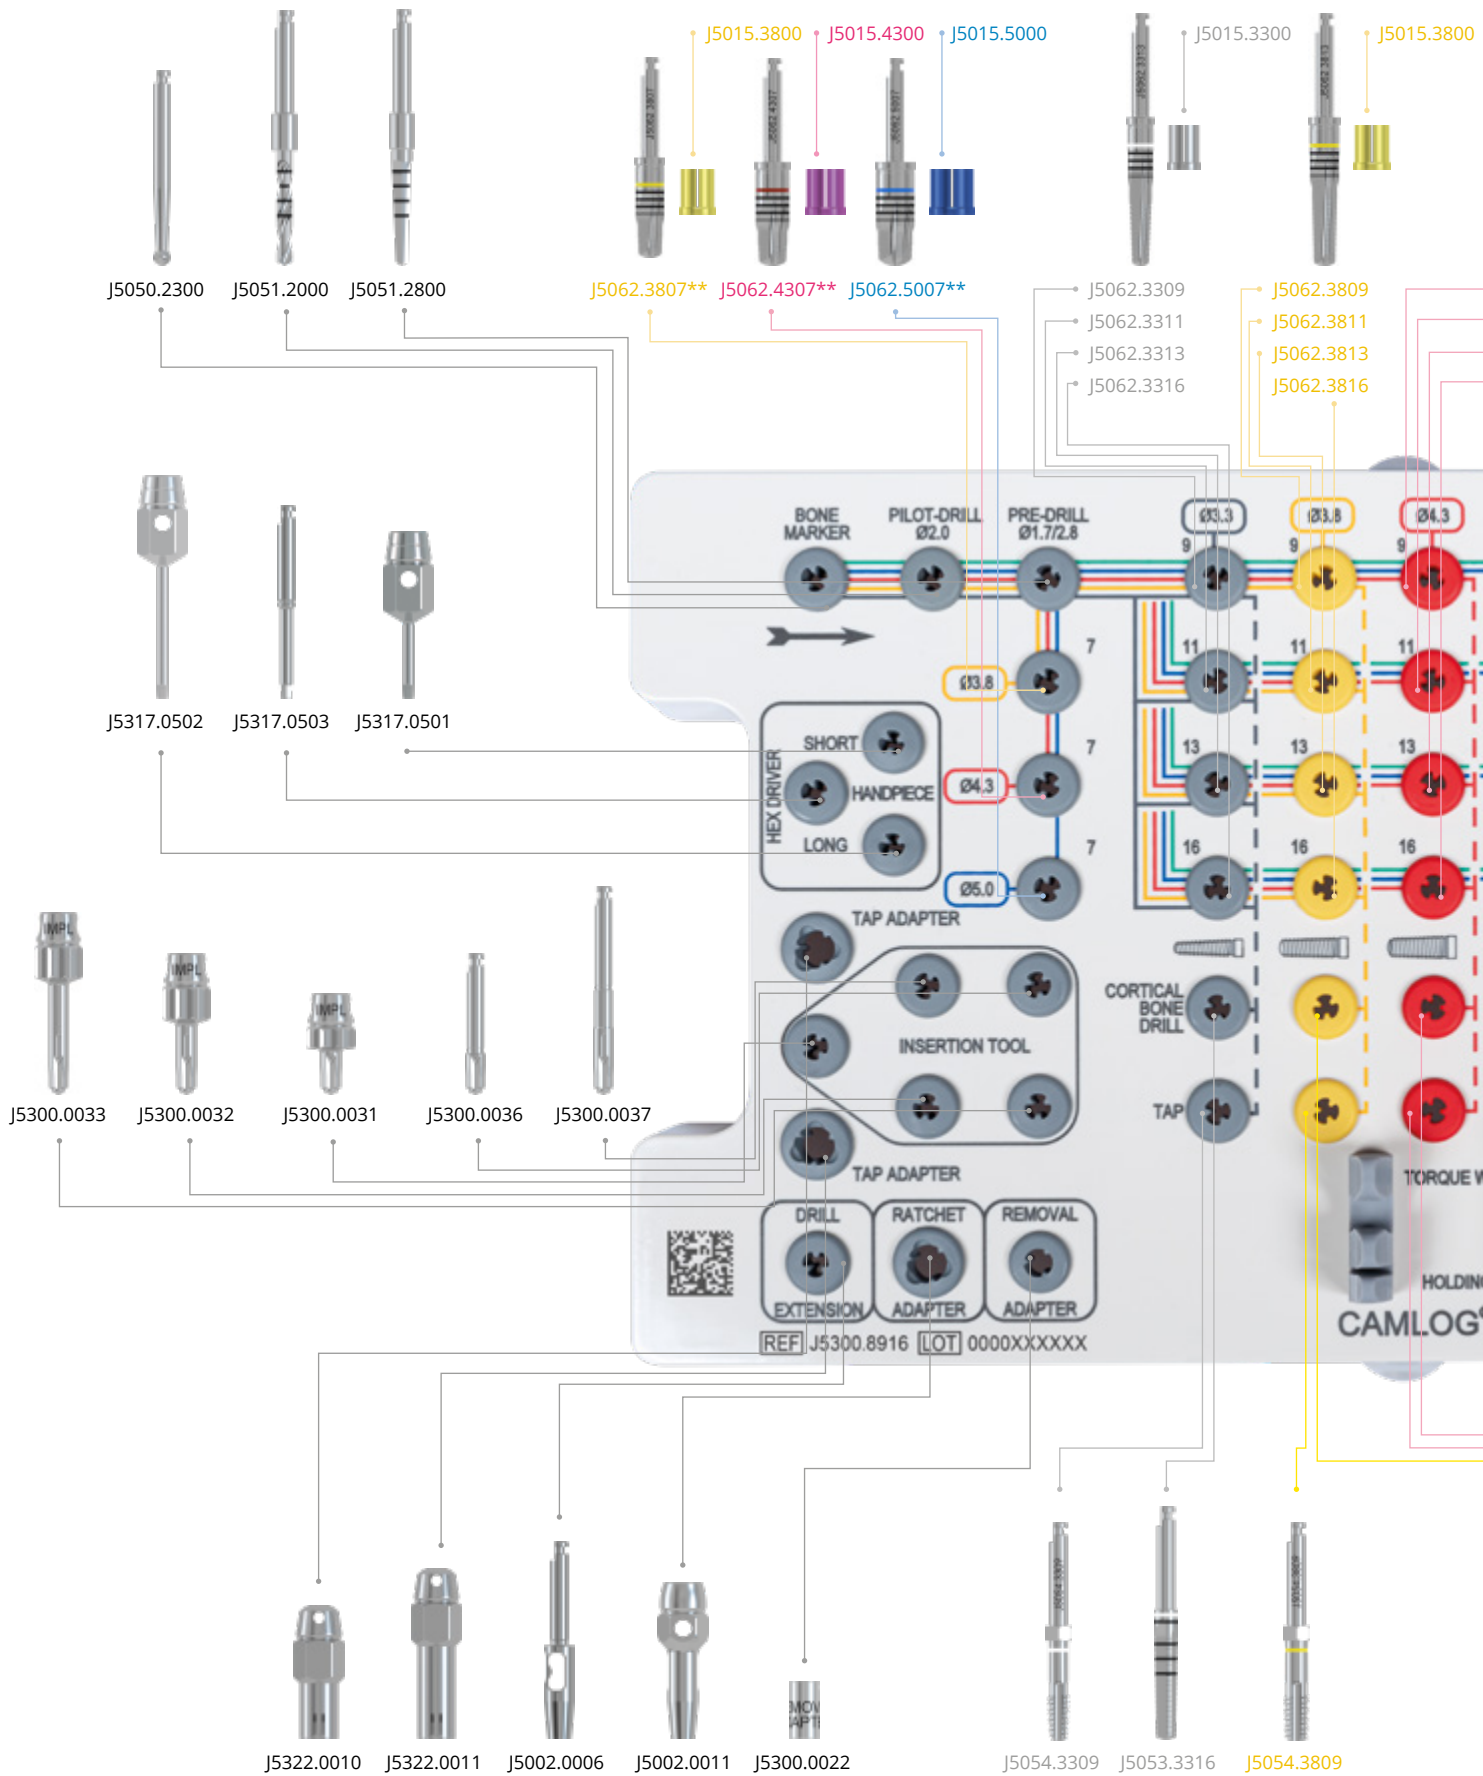

\* This article is not included in the surgery set and must be ordered separately.

**Note**

- The drills are arranged and sorted in the set according to the treatment sequence.
- Colored lines indicate the exact drilling sequence.

J5015.4300 J5015.5000 J5015.6000\*

J5062.4309 J5062.4311 J5062.4313 J5062.4316 J5062.5009 J5062.5011 J5062.5013 J5062.5016 J5062.6009\* J5062.6011\* J5062.6013\* J5062.6016\*

J5300.2028

J5015.0013 J5015.0011 J5015.0009 J5015.0007

J5320.1030

J5302.0010

J5053.3816 J5054.4309 J5053.4316 J5054.5009 J5053.5016 J5054.6009\* J5053.6016\*





# SCREW-LINE

## Surgery set and wash tray

	Article	Art. No.
 <p>A white plastic surgery set tray containing various surgical instruments. The instruments are organized into rows and color-coded: blue, yellow, red, and green. A torque wrench and a universal holding key are also visible on the right side of the tray. The tray is labeled 'CAMLOG®/CONELOG® SCREW-LINE'.</p>	<p><b>Surgery Set</b>  <b>CAMLOG®/CONELOG®</b>  <b>SCREW-LINE</b>            contains all necessary color-code ordered surgical instruments, incl. torque wrench and universal holding key (drills and taps for Ø 6.0 mm are not included)</p>	<p>J5300.0063</p>
 <p>A rectangular metal wash tray with a grid of circular holes. The holes are color-coded to match the surgical instruments in the set. The tray is labeled 'CAMLOG®/CONELOG® SCREW-LINE' and includes a QR code.</p>	<p><b>Surgery wash tray</b>  <b>CAMLOG®/CONELOG®</b>  <b>SCREW-LINE</b>            incl. pattern, without content</p>	<p>J5300.8968</p>
 <p>A metal pattern for the wash tray, showing the layout of the holes. The holes are color-coded and labeled with numbers 1 through 11. The pattern is labeled 'CAMLOG®/CONELOG® SCREW-LINE' and includes a QR code.</p>	<p><b>Pattern for surgery wash tray</b>  <b>CAMLOG®/CONELOG®</b>  <b>SCREW-LINE</b>    <b>Material</b>            Stainless steel</p>	<p>J5300.1073</p>




Preparation of the implant bed for CAMLOG® SCREW-LINE Implants and for CONELOG® SCREW-LINE Implants is performed with identical instruments.

## Surgical instruments

	Article	Art. No.	Ø	L
	<b>Form drills</b> <b>SCREW-LINE</b> resterilizable  <b>Material</b> Stainless steel	J5062.3309	3.3 mm	9 mm
		J5062.3311		11 mm
		J5062.3313		13 mm
		J5062.3316		16 mm
		J5062.3807	3.8 mm	7 mm
		J5062.3809		9 mm
		J5062.3811		11 mm
		J5062.3813		13 mm
		J5062.3816	16 mm	
		J5062.4307	4.3 mm	7 mm
		J5062.4309		9 mm
		J5062.4311		11 mm
		J5062.4313		13 mm
		J5062.4316	16 mm	
		J5062.5007	5.0 mm	7 mm
		J5062.5009		9 mm
		J5062.5011		11 mm
		J5062.5013		13 mm
J5062.5016	16 mm			
	<b>Depth stop, for form drills</b> <b>PROGRESSIVE-LINE and SCREW-LINE</b> resterilizable  <b>Material</b> Titanium alloy	J5015.3300	3.3 mm	-
		J5015.3800	3.8 mm	
		J5015.4300	4.3 mm	
		J5015.5000	5.0 mm	
	<b>Form drills</b> <b>SCREW-LINE cortical bone,</b> resterilizable  <b>Material</b> Stainless steel	J5053.3316	3.3 mm	-
		J5053.3816	3.8 mm	
		J5053.4316	4.3 mm	
		J5053.5016	5.0 mm	
	<b>Tap</b> <b>SCREW-LINE</b> with hexagon, resterilizable  <b>Material</b> Stainless steel	J5054.3309	3.3 mm	-
		J5054.3809	3.8 mm	
		J5054.4309	4.3 mm	
		J5054.5009	5.0 mm	

# SCREW-LINE

## Surgical instruments

	Article	Art. No.	Ø	L
	<p><b>EP pilot drill set</b> sterile</p> <p><b>Content:</b> EP round bur (Ø 3.0 mm) EP pilot drill (Ø 2.0 mm)</p> <p><b>Material</b> Stainless steel / plastic</p>	J5060.0001	-	-
	<p><b>SCREW-LINE EP pre-drill</b> sterile</p> <p><b>Material</b> Stainless steel / plastic</p>	J5060.2800	1.7– 2.8 mm	-
	<p><b>SCREW-LINE EP form drill</b> sterile</p> <p><b>Material</b> Stainless steel / plastic</p>	J5060.3309	3.3 mm	9 mm
		J5060.3311		11 mm
		J5060.3313		13 mm
		J5060.3807	3.8 mm	7 mm
		J5060.3809		9 mm
		J5060.3811		11 mm
		J5060.3813		13 mm
		J5060.4307	4.3 mm	7 mm
		J5060.4309		9 mm
		J5060.4311		11 mm
		J5060.4313	13 mm	
		J5060.5007	5.0 mm	7 mm
		J5060.5009		9 mm
		J5060.5011		11 mm
J5060.5013	13 mm			

EP: Single-patient drill



The EP drills are for single use only and must not be resterilized.

# SCREW-LINE Guide System



# SCREW-LINE Guide System

## Surgical instruments

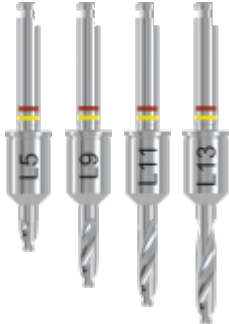	Article	Art. No.	Ø	L
	<b>Guide System Pilot drill set</b> internal irrigation, sterile (for pilot drilling Ø 2.0 mm)  <b>Material</b> Stainless steel	J5063.3309	3.3 mm	9 mm (incl. 5 mm)**
		J5063.3311		11 mm (incl. 5 and 9 mm)**
		J5063.3313		13 mm (incl. 5, 9 and 11 mm)**
		J5064.3316*		16 mm
		J5063.4307	3.8 mm	7 mm (incl. 5 mm)**
			4.3 mm	
		J5063.4309	3.8 mm	9 mm (incl. 5 mm)**
			4.3 mm	
		J5063.4311	3.8 mm	11 mm (incl. 5 and 9 mm)**
			4.3 mm	
J5063.4313	3.8 mm	13 mm (incl. 5, 9 and 11 mm)**		
	4.3 mm			
J5064.4316*	3.8 mm	16 mm		
	4.3 mm			
	<b>Guide System Surgery Set SCREW-LINE</b> internal irrigation, sterile  <b>Material</b> Stainless steel	J5065.3309	3.3 mm	9 mm (incl. 5 mm)****
		J5065.3311		11 mm (incl. 5 and 9 mm)****
		J5065.3313		13 mm (incl. 5, 9 and 11 mm)****
		J5066.3316****		16 mm
		J5065.3807	3.8 mm	7 mm (incl. 5 mm)****
		J5065.3809		9 mm (incl. 5 mm)****
		J5065.3811		11 mm (incl. 5 and 9 mm)****
		J5065.3813		13 mm (incl. 5, 9 and 11 mm)****
		J5066.3816****	16 mm	
		J5065.4307	4.3 mm	7 mm (incl. 5 mm)****
		J5065.4309		9 mm (incl. 5 mm)****
		J5065.4311		11 mm (incl. 5 and 9 mm)****
		J5065.4313		13 mm (incl. 5, 9 and 11 mm)****
		J5066.4316****		16 mm

\* Necessary Guide System pilot drill for implant length 16 mm, following obligatory prior use of the pilot drill set length 13 mm.

\*\* All Guide System pilot drill sets include a 5 mm long pilot drill, as well as all pilot drills necessary for the selected implant length.

\*\*\* Necessary Guide System form drill for implant length 16 mm, following obligatory prior use of the Guide System surgery set length 13 mm.





\*\*\*\* All Guide System surgery sets include a 5 mm long pre-drill, as well as all form drills necessary for the selected implant length.

All Guide System drills and gingiva punches for SCREW-LINE are intended for single use only.

### Note

Implants with the screw-mounted insertion post (Art. No. C10655.xxxx) are to be used for template-guided implant insertion with the SCREW-LINE Guide System. The SCREW-LINE Guide System can only be used for implant diameters 3.3/3.8/4.3 mm.



	Article	Art. No.	Ø	L
	<b>Guide System</b> <b>Form drill SCREW-LINE</b> <b>cortical bone</b> internal irrigation, sterile  <b>Material</b> Stainless steel	J5068.3309	3.3 mm	9 mm
		J5068.3311		11 mm
		J5068.3313		13 mm
		J5068.3316		16 mm
		J5068.3807	3.8 mm	7 mm
		J5068.3809		9 mm
		J5068.3811		11 mm
		J5068.3813		13 mm
		J5068.3816		16 mm
		J5068.4307		4.3 mm
		J5068.4309	9 mm	
		J5068.4311	11 mm	
		J5068.4313	13 mm	
		J5068.4316	16 mm	
	<b>Guide System</b> <b>Gingiva punch</b> sterile  <b>Material</b> Stainless steel	J5041.3303	3.3 mm	-
		J5041.3803	3.8 mm	
		J5041.4303	4.3 mm	
	<b>Guide System</b> <b>guiding sleeve</b> Height 3.0 mm (2 units)  <b>Material</b> Titanium alloy	J3734.3303*	3.3 mm	-
		J3734.3803*	3.8 mm	
		J3734.4303*	4.3 mm	
	<b>Drill extension</b> ISO shaft, for instruments with internal irrigation  <b>Material</b> Stainless steel	J5002.0005	-	26.6 mm






\* The sleeves are not compatible with the PROGRESSIVE-LINE Guide System.

All Guide System drills and gingiva punches for SCREW-LINE are intended for single use only.






# General surgical instruments



## General surgical instruments

	Article	Art. No.	Ø	L
	<p><b>Round bur</b> resterilizable</p> <p><b>Material</b> Stainless steel</p>	J5050.2300	2.3 mm	-
	<p><b>Point drill</b> resterilizable</p> <p><b>Material</b> Stainless steel</p>	J5051.1500	1.5 mm	-
	<p><b>Pilot drill</b> without coil, resterilizable</p> <p><b>Material</b> Stainless steel</p>	J5051.2003	2.0 mm	-
	<p><b>Pilot drill SCREW-LINE</b> resterilizable</p> <p><b>Material</b> Stainless steel</p>	J5051.2000	2.0 mm	-
	<p><b>Pre-drill SCREW-LINE</b> resterilizable</p> <p><b>Material</b> Stainless steel</p>	J5051.2800	1.7–2.8 mm	-

# General surgical instruments








	Article		Art. No.	Ø	L
	<b>Depth stop SCREW-LINE</b> for pilot drill (J5051.2000) and pre-drill (J5051.2800), resterilizable  <b>Material</b> Stainless steel		J5015.0009	-	9 mm
			J5015.0011		11 mm
			J5015.0013		13 mm
	<b>Bone profiler</b>  <b>Material</b> Stainless steel	Ø 5.0 mm	J5003.3350*	3.3 mm	-
		Ø 6.0 mm	J5003.4360*	3.8 mm	
				4.3 mm	
		Ø 7.0 mm	J5003.5070*	5.0 mm	
	<b>CONELOG® Guiding pin for bone profiler</b>  <b>Material</b> Titanium alloy		C5002.3300	3.3 mm	-
			C5002.3800	3.8 mm	
			C5002.4300	4.3 mm	
			C5002.5000	5.0 mm	
	<b>Countersink</b>  <b>Material</b> Stainless steel	Ø 4.6 mm	J5006.3346	3.3 mm	-
		Ø 5.2 mm	J5006.3852	3.8 mm	
		Ø 5.6 mm	J5006.4356	4.3 mm	
		Ø 6.3 mm	J5006.5063	5.0 mm	
	<b>Baring drill for cover screw</b>  <b>Material</b> Stainless steel		J5004.3300	3.3 mm	-
			J5004.3800	3.8 mm	
			J5004.4300	4.3 mm	
			J5004.5000	5.0 mm	

\* Always to be used in conjunction with the matching guiding pin!

	Article	Art. No.	∅	Dimension
	<b>Paralleling pin SCREW-LINE</b> with depth marks  <b>Material</b> Titanium alloy	J5300.2028	-	∅ 1.7-2.8 mm/ 2.0 mm
	<b>Drill extension</b> ISO shaft (not for drills with internal irrigation)  <b>Material</b> Stainless steel	J5002.0006	-	26.5 mm
	<b>Tap adapter, short</b> for tap SCREW-LINE  <b>Material</b> Stainless steel	J5322.0010	-	18.0 mm
	<b>Tap adapter, long</b> for tap SCREW-LINE  <b>Material</b> Stainless steel	J5322.0011	-	23.0 mm
	<b>Removal adapter</b> <b>for CAMLOG® and CONELOG®</b> suitable for all implant diameters  <b>Material</b> Stainless steel	J5300.0022*	3.3 mm 3.8 mm 4.3 mm 5.0 mm	6.2 mm

\* only for use with CONELOG® PROGRESSIVE-LINE Implants with Art. No. C1086.xxxx as well as CONELOG® SCREW-LINE Implants with Art. No. C1066.xxxx








# General surgical instruments

	Article	Art. No.	Dimension
	<b>Insertion tool, extra short</b> for screw implants, manual/wrench  <b>Material</b> Stainless steel	J5300.0031*	13.7 mm
	<b>Insertion tool, short</b> for screw implants, manual/wrench  <b>Material</b> Stainless steel	J5300.0032*	19.2 mm
	<b>Insertion tool, long</b> for screw implants, manual/wrench  <b>Material</b> Stainless steel	J5300.0033*	24.8 mm
	<b>Insertion tool, short</b> for screw implants, with ISO-shaft for angled hand piece (without hexagon at the shaft)  <b>Material</b> Stainless steel	J5300.0036*	19.1 mm
	<b>Insertion tool, long</b> for screw implants, with ISO-shaft for angled hand piece (without hexagon at the shaft)  <b>Material</b> Stainless steel	J5300.0037*	28.2 mm
	<b>Insertion tool, short</b> for screw implants, with ISO-shaft for angled hand piece, for hex clamping system  <b>Material</b> Stainless steel	J5300.0034*	19.1 mm
	<b>Insertion tool, long</b> for screw implants, with ISO-shaft for angled hand piece, for hex clamping system  <b>Material</b> Stainless steel	J5300.0035*	28.2 mm






\* only for use with CONELOG® PROGRESSIVE-LINE Implants with Art. No. C1085.xxxx and C1086.xxxx as well as CONELOG® SCREW-LINE Implants with Art. No. C1065.xxxx and C1066.xxxx

	Article	Art. No.	Dimension
	<p><b>Torque wrench</b> with continuous torque adjustment until maximal 30 Ncm</p> <p><b>Material</b> Stainless steel</p>	J5320.1030	-
	<p><b>PickUp instrument</b> holder for carrying implants</p> <p><b>Material</b> Stainless steel</p>	J5300.0030	-
	<p><b>Adapter</b> ISO shaft for angled hand piece/wrench</p> <p><b>Material</b> Stainless steel</p>	J5002.0011	21.0 mm

# General surgical instruments

	Article	Art. No.	Ø	Dimension
	<b>Universal holding key</b>  <b>Material</b> Stainless steel	J5302.0010	-	-
	<b>CONELOG® Insertion aid, short</b> for CONELOG® Implants  <b>Material</b> Stainless steel	C5302.3311	3.3 mm	28.1 mm
		C5302.4311	3.8 mm	
		C5302.5011	4.3 mm	
	<b>CONELOG® Insertion aid, long</b> for CONELOG® Implants  <b>Material</b> Stainless steel	C5302.3310	3.3 mm	33.1 mm
		C5302.4310	3.8 mm	
		C5302.5010	4.3 mm	
	<b>Sleeve for inserting the insertion aid into the implant</b> color-coded  <b>Material</b> Titanium alloy	J5302.3300	3.3 mm	-
		J5302.3800	3.8 mm	
		J5302.4300	4.3 mm	
		J5302.5000	5.0 mm	
	<b>Screwdriver</b> hex, extra short, manual/wrench  <b>Material</b> Stainless steel	J5317.0510	-	14.5 mm
	<b>Screwdriver</b> hex, short, manual/wrench  <b>Material</b> Stainless steel	J5317.0501	-	22.5 mm
	<b>Screwdriver</b> hex, long, manual/wrench  <b>Material</b> Stainless steel	J5317.0502	-	30.3 mm




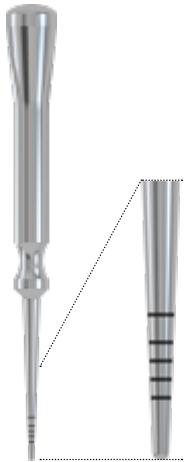
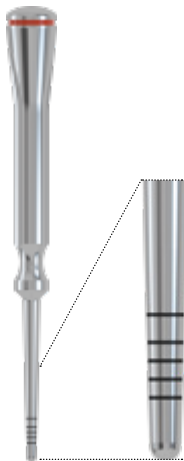
	Article	Art. No.	Dimension
	<b>Screwdriver</b> hex, short, ISO shaft  <b>Material</b> Stainless steel	J5317.0504	18.0 mm
	<b>Screwdriver</b> hex, long, ISO shaft  <b>Material</b> Stainless steel	J5317.0503	26.0 mm
	<b>Manual screwdriver, hex</b> without wrench head connection  <b>Material</b> Stainless steel	J5317.0511	23.0 mm
	<b>Cleaning needle</b> for instruments with internal irrigation  <b>Material</b> Stainless steel	J5002.0012	-
	<b>Cleaning cannula</b> for instruments with internal irrigation  <b>Material</b> Stainless steel	J5002.0020	-

# SCREW-LINE Osteotomy Set



# SCREW-LINE Osteotomy Set

straight convex


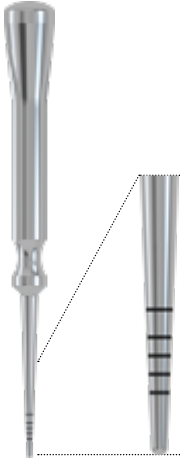
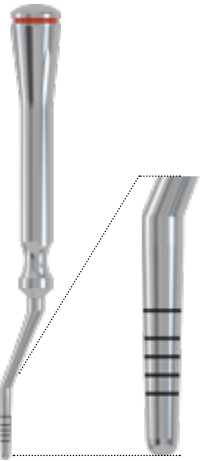
	Article	Art. No.	Ø
	<p><b>Osteotomy Set</b>  <b>CAMLOG®/CONELOG® SCREW-LINE</b>            straight convex</p> <p><b>Material</b>            Stainless steel</p>	<p>J5418.0020</p>	<p>-</p>
	<p><b>Pre-Osteotome SCREW-LINE</b>            straight convex</p> <p><b>Material</b>            Stainless steel</p>	<p>J5417.2800*</p>	<p>1.7– 2.8 mm</p>
	<p><b>Osteotome SCREW-LINE</b>            straight convex</p> <p><b>Material</b>            Stainless steel</p>	<p>J5418.3300*            J5418.3800*            J5418.4300*            J5418.5000*</p>	<p>3.3 mm            3.8 mm            4.3 mm            5.0 mm</p>

\* These products are included in the CAMLOG®/CONELOG® SCREW-LINE straight-convex osteotomy set.

Surgery




# SCREW-LINE Osteotomy Set

angled convex

	Article	Art. No.	Ø
	<p><b>Osteotomy Set</b>  <b>CAMLOG®/CONELOG® SCREW-LINE</b>            angled convex</p> <p><b>Material</b>            Stainless steel</p>	<p>J5418.0030</p>	<p>-</p>
	<p><b>Pre-Osteotome SCREW-LINE</b>            straight convex</p> <p><b>Material</b>            Stainless steel</p>	<p>J5417.2800*</p>	<p>1.7– 2.8 mm</p>
	<p><b>Osteotome SCREW-LINE</b>            angled convex</p> <p><b>Material</b>            Stainless steel</p>	<p>J5418.3310*</p> <p>J5418.3810*</p> <p>J5418.4310*</p> <p>J5418.5010*</p>	<p>3.3 mm</p> <p>3.8 mm</p> <p>4.3 mm</p> <p>5.0 mm</p>

\* These products are included in the CAMLOG®/CONELOG® SCREW-LINE angled-convex osteotomy set.


straight concave

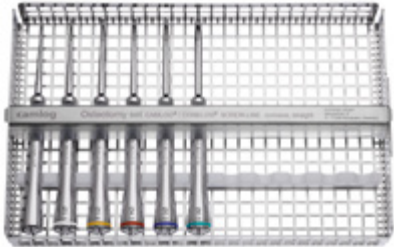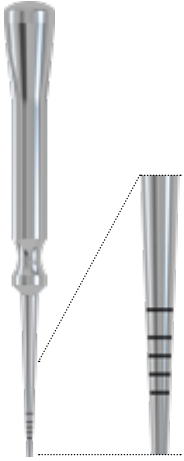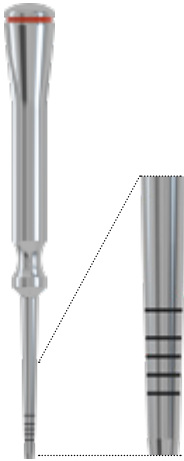	Article	Art. No.	Ø								
	<p><b>Osteotomy Set</b>  <b>CAMLOG®/CONELOG® SCREW-LINE</b>                      straight concave</p> <p><b>Material</b>                      Stainless steel</p>	J5420.0020	-								
	<p><b>Pre-Osteotome SCREW-LINE</b>                      straight concave</p> <p><b>Material</b>                      Stainless steel</p>	J5419.2800*	1.7– 2.8 mm								
	<p><b>Osteotome SCREW-LINE</b>                      straight concave</p> <p><b>Material</b>                      Stainless steel</p>	<table border="1"> <tr> <td data-bbox="1193 1272 1361 1402">J5420.3300*</td> <td data-bbox="1361 1272 1476 1402">3.3 mm</td> </tr> <tr> <td data-bbox="1193 1402 1361 1532">J5420.3800*</td> <td data-bbox="1361 1402 1476 1532">3.8 mm</td> </tr> <tr> <td data-bbox="1193 1532 1361 1662">J5420.4300*</td> <td data-bbox="1361 1532 1476 1662">4.3 mm</td> </tr> <tr> <td data-bbox="1193 1662 1361 1783">J5420.5000*</td> <td data-bbox="1361 1662 1476 1783">5.0 mm</td> </tr> </table>	J5420.3300*	3.3 mm	J5420.3800*	3.8 mm	J5420.4300*	4.3 mm	J5420.5000*	5.0 mm	
J5420.3300*	3.3 mm										
J5420.3800*	3.8 mm										
J5420.4300*	4.3 mm										
J5420.5000*	5.0 mm										

\* These products are included in the CAMLOG®/CONELOG® SCREW-LINE straight-concave osteotomy set.

# SCREW-LINE Osteotomy Set

angled concave

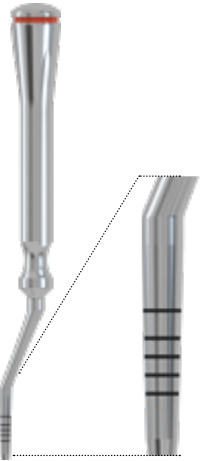
	Article	Art. No.	Ø
	<b>Osteotomy Set</b> <b>CAMLOG®/CONELOG® SCREW-LINE</b> angled concave  <b>Material</b> Stainless steel	J5420.0030	-
	<b>Pre-Osteotome SCREW-LINE</b> straight concave  <b>Material</b> Stainless steel	J5419.2800*	1.7– 2.8 mm
	<b>Osteotome SCREW-LINE</b> angled concave  <b>Material</b> Stainless steel	J5420.3310*	3.3 mm
		J5420.3810*	3.8 mm
		J5420.4310*	4.3 mm
		J5420.5010*	5.0 mm

\* These products are included in the CAMLOG®/CONELOG® SCREW-LINE angled-concave osteotomy set.

# Cover screws and healing caps






## Cover screws

	Article	Art. No.	Ø
	<b>CONELOG® Implant cover screw</b>  <b>Material</b> Titanium alloy	C2019.3300	3.3 mm
		C2019.3800	3.8 mm
		C2019.4300	4.3 mm
		C2019.5000	5.0 mm

The implant cover screws are for single use only and must not be resterilized.

## Healing caps

	Article	Art. No.	Ø	GH	G Ø
	<b>CONELOG® Healing cap, cylindrical</b> sterile  <b>Material</b> Titanium alloy	C2015.3320	3.3 mm	2.0 mm	3.0 mm
		C2015.3340		4.0 mm	3.0 mm
		C2015.3820	3.8 mm	2.0 mm	3.5 mm
		C2015.3840		4.0 mm	3.5 mm
		C2015.3860*	6.0 mm	3.5 mm	
		C2015.4320	4.3 mm	2.0 mm	3.8 mm
		C2015.4340		4.0 mm	3.8 mm
		C2015.4360*		6.0 mm	3.8 mm
		C2015.5020	5.0 mm	2.0 mm	4.5 mm
		C2015.5040		4.0 mm	4.5 mm
C2015.5060*	6.0 mm	4.5 mm			
	<b>CONELOG® Healing cap, wide body</b> sterile  <b>Material</b> Titanium alloy	C2014.3340	3.3 mm	4.0 mm	4.8 mm
		C2014.3840	3.8 mm	4.0 mm	5.3 mm
		C2014.3860		6.0 mm	5.3 mm
		C2014.4340	4.3 mm	4.0 mm	5.8 mm
		C2014.4360		6.0 mm	5.8 mm
		C2014.5040	5.0 mm	4.0 mm	6.5 mm
C2014.5060	6.0 mm	6.5 mm			
	<b>CONELOG® Healing cap, bottleneck</b> sterile  <b>Material</b> Titanium alloy	C2011.3340	3.3 mm	4.0 mm	3.3 mm
		C2011.3840	3.8 mm	4.0 mm	3.8 mm
		C2011.3860		6.0 mm	3.8 mm
		C2011.4340	4.3 mm	4.0 mm	4.0 mm
		C2011.4360		6.0 mm	4.0 mm
		C2011.5040	5.0 mm	4.0 mm	4.7 mm
C2011.5060	6.0 mm	4.7 mm			

\* suitable for bite registration



Healing caps are for single use only and must not be resterilized.



# Prosthetics



# Scanbodies

	Article	Art. No.	Ø
	<p><b>CONELOG® Scanbody*</b> for optical, 3-dimensional localization of CONELOG® Implants in the mouth or CONELOG® Lab analogs in the working model, incl. abutment screw, sterile</p> <p>Not compatible with the CEREC and inLab systems from Dentsply Sirona</p> <p><b>Material</b> PEEK</p>	C2600.3310	3.3 mm
		C2600.4310	3.8 mm
			4.3 mm
		C2600.5010	5.0 mm
	<p><b>CONELOG® ScanPost for Sirona® Scanbody</b> for digital recording of the CONELOG® Implant or lab analog position and for further processing in the CEREC and inLab systems from Dentsply Sirona, incl. abutment screw</p> <p><b>Material</b> Titanium alloy</p>	C2620.3306	3.3 mm
		C2620.3806	3.8 mm
		C2620.4306	4.3 mm
		C2620.5006	5.0 mm

\* Please check whether the CONELOG® Scanbody is available in the CAD software used.  
CAD libraries for selected CONELOG® Prosthetic components are available for free download here:  
[www.camlog.com/en/media-center/cad-libraries](http://www.camlog.com/en/media-center/cad-libraries)

**Matching Sirona® Scanbodies size S for CONELOG® ScanPost and CONELOG® Titanium base CAD/CAM, crown, with Ø 3.3/3.8/4.3 mm:**




For Omnicam®: Article number 6431311  
For Bluecam®: Article number 6431295

**Matching Sirona® Scanbodies size L for CONELOG® ScanPost and CONELOG® Titanium base CAD/CAM, crown, with Ø 5.0 mm:**



For Omnicam®: Article number 6431329  
For Bluecam®: Article number 6431303

Sirona® Scanbodies are available from Dentsply Sirona.






# Impression taking

	Article	Art. No.	Ø
 <p>3 mm 10 mm</p>	<b>CONELOG® Impression post, open tray</b> incl. fixing screw (the fixing screw can be shortened extra-oral by 3 mm with a screwdriver, hex)  <b>Material</b> Titanium alloy	C2121.3300	3.3 mm
		C2121.3800	3.8 mm
		C2121.4300	4.3 mm
		C2121.5000	5.0 mm
 <p>10.7 mm</p>	<b>CONELOG® Impression post, closed tray</b> incl. impression cap, bite registration cap and fixing screw  <b>Material</b> Titanium alloy / POM	C2110.3300	3.3 mm
		C2110.3800	3.8 mm
		C2110.4300	4.3 mm
		C2110.5000	5.0 mm
	<b>Impression cap for impression post, closed tray</b> (5 units)  <b>Material</b> POM	J2111.3300	3.3 mm
		J2111.3800	3.8 mm
		J2111.4300	4.3 mm
		J2111.5000	5.0 mm

## Bite registration



	Article	Art. No.	Ø
	<b>CONELOG® Bite registration post</b> incl. fixing screw and bite registration cap  <b>Material</b> Titanium alloy / POM	C2140.3300	3.3 mm
		C2140.3800	3.8 mm
		C2140.4300	4.3 mm
		C2140.5000	5.0 mm
	<b>Bite registration cap</b> (5 units)  <b>Material</b> POM	J2112.3300	3.3 mm
		J2112.3800	3.8 mm
		J2112.4300	4.3 mm
		J2112.5000	5.0 mm

## Cast fabrication

	Article	Art. No.	Ø
	<b>CONELOG® Lab analog</b> for cast models  <b>Material</b> Titanium alloy	C3010.3300	3.3 mm
		C2211.3300	3.8 mm
		C3010.4300	4.3 mm
		C3010.5000	5.0 mm
	<b>CONELOG® Lab analog (3 units)</b> for cast models  <b>Material</b> Titanium alloy	C3010.3303	3.3 mm
		C3010.3803	3.8 mm
		C3010.4303	4.3 mm
		C3010.5003	5.0 mm
	<b>CONELOG® Implant analog</b> for printed and cast models  <b>Material</b> Titanium alloy	C3025.3300	3.3 mm
		C3025.3800	3.8 mm
		C3025.4300	4.3 mm
		C3025.5000	5.0 mm
	<b>CONELOG® Implant analog (3 units)</b> for printed and cast models  <b>Material</b> Titanium alloy	C3025.3303	3.3 mm
		C3025.3803	3.8 mm
		C3025.4303	4.3 mm
		C3025.5003	5.0 mm
	<b>DIM Analog® for the CONELOG® Implant System</b> for printed models, incl. knurled nut  <b>Material</b> Titanium alloy / stainless steel	C3012.3300	3.3 mm
		C3012.4300	3.8 mm
			4.3 mm
C3012.5000	5.0 mm		

Manufacturer DIM Analog®: NT-Trading GmbH & Co. KG | G.-Braun-Straße 18 | 76187 Karlsruhe | Germany  
 DIM Analog® is a registered trademark of the NT-Trading GmbH & Co. KG company.





# Temporary abutments

	Article	Art. No.	Ø	GH
 <p>11 mm</p>	<b>CONELOG® Temporary abutment, crown, titanium alloy</b> preparable, incl. abutment screw  <b>Material</b> Titanium alloy	C2239.3300*	3.3 mm	-
		C2239.3800	3.8 mm	
		C2239.4300	4.3 mm	
		C2239.5000	5.0 mm	
 <p>11.2 mm</p>	<b>CONELOG® Temporary abutment, bridge, titanium alloy</b> preparable, incl. abutment screw  <b>Material</b> Titanium alloy	C2339.3300	3.3 mm	-
		C2339.3800	3.8 mm	
		C2339.4300	4.3 mm	
		C2339.5000	5.0 mm	

\* only for crown restorations in the region of the upper lateral and lower lateral and central incisors

# CAD/CAM prosthetics

## Crown, bridge and hybrid restoration

	Article	Art. No.	Ø	GH
	<b>CONELOG® Titanium base CAD/CAM, crown</b> Bonding base for individual CAD/CAM fabricated dental prostheses, incl. dark purple anodized abutment screw and bonding aid (POM)  <b>Material</b> Titanium alloy / POM	C2242.3308*	3.3 mm	0.8 mm
		C2242.3808	3.8 mm	
		C2242.4308	4.3 mm	
		C2242.5008	5.0 mm	
	<b>CONELOG® Titanium base CAD/CAM, crown</b> Bonding base for individual CAD/CAM fabricated dental prostheses, incl. dark purple anodized abutment screw and bonding aid (POM)  <b>Material</b> Titanium alloy / POM	C2242.3320*	3.3 mm	2.0 mm
		C2242.3820	3.8 mm	
		C2242.4320	4.3 mm	
		C2242.5020	5.0 mm	
	<b>CONELOG® Titanium base CAD/CAM, bridge</b> Bonding base for individual CAD/CAM fabricated dental prostheses, incl. dark purple anodized abutment screw and bonding aid (POM)  <b>Material</b> Titanium alloy / POM	C2342.3308	3.3 mm	0.8 mm
		C2342.3808	3.8 mm	
		C2342.4308	4.3 mm	
		C2342.5008	5.0 mm	
	<b>CONELOG® Titanium base CAD/CAM, bridge</b> Bonding base for individual CAD/CAM fabricated dental prostheses, incl. dark purple anodized abutment screw and bonding aid (POM)  <b>Material</b> Titanium alloy / POM	C2342.3320	3.3 mm	2.0 mm
		C2342.3820	3.8 mm	
		C2342.4320	4.3 mm	
		C2342.5020	5.0 mm	




\* only for crown restorations in the region of the upper lateral and lower lateral and central incisors

The geometries of the CONELOG® Titanium bases CAD/CAM are available as a CAD library for leading dental CAD systems.

The libraries are available for free download at:  
[www.camlog.com/en/media-center/cad-libraries](http://www.camlog.com/en/media-center/cad-libraries)




### DEDICAM® CAD/CAM prosthetics from Camlog

Find out more about DEDICAM® Products at your appropriate Camlog country representative.

	Article	Art. No.	Ø	Thread
	<b>CONELOG® Modeling aid for CONELOG® Titanium base CAD/CAM, crown burn-out, for fabricating mesostructures and crowns</b>  <b>Material</b> POM	C2242.3302	3.3 mm	-
		C2242.3802	3.8 mm	
		C2242.4302	4.3 mm	
		C2242.5002	5.0 mm	
	<b>CONELOG® Abutment screw for CONELOG® Titanium base CAD/CAM dark purple anodized</b>  <b>Material</b> Titanium alloy	C4015.1601	3.3 mm	M1.6
			3.8 mm	
			4.3 mm	
		C4015.2001	5.0 mm	M2.0
	<b>CONELOG® Lab screw for CONELOG® Titanium base CAD/CAM partially brown anodized</b>  <b>Material</b> Titanium alloy	C4016.1601	3.3 mm	M1.6
			3.8 mm	
			4.3 mm	
		C4016.2001	5.0 mm	M2.0

# CAM blanks

## Milling of customized, one-piece abutments and healing caps using CAD/CAM technology

	Article	Art. No.	Ø
	<b>CONELOG® CAM titanium blank, type IAC**</b> Ø 12 mm, length 12.5 mm (2 units), Shipping incl. 2 separately packed abutment screws  <b>Material</b> Titanium alloy	C2431.3313*	3.3 mm
		C2431.3813	3.8 mm
		C2431.4313	4.3 mm
		C2431.5013	5.0 mm
	<b>CONELOG® CAM titanium blank, type ME***</b> Ø 12 mm, length 20 mm (2 units), Shipping incl. 2 separately packed abutment screws  <b>Material</b> Titanium alloy	C2441.3320*	3.3 mm
		C2441.3820	3.8 mm
		C2441.4320	4.3 mm
		C2441.5020	5.0 mm
	<b>CONELOG® CAM CoCr blank, type ME***</b> Ø 12 mm, length 20 mm (2 units), Shipping incl. 2 separately packed abutment screws  <b>Material</b> Cobalt chrome alloy	C2461.3320*	3.3 mm
		C2461.4320	3.8 mm
			4.3 mm
		C2461.5020	5.0 mm

\* only for crown restorations in the region of the upper lateral and lower lateral and central incisors (Ø 3.3 mm not for double crown restorations)

\*\* Type IAC

For the milling process, the CAM titanium blank, type IAC is fixated to the implant-abutment connection via the CONELOG® Collet for CAM blanks. The machine-specific holders and adapters for the collet as well as the milling strategies are to be provided by the user.

\*\*\* Type ME

For the milling process, the CAM blank, type ME is fixed to a cylindrical section opposite the implant-abutment connection. Medentika® Preface® Abutment holders can be used as machine-specific clamping devices. These collets are available for selected machines from the respective machine manufacturers. The milling strategies are to be provided by the user.


The geometries of the CONELOG® CAM blanks are available as a CAD library for leading dental CAD systems.

The libraries are available for free download at:  
[www.camlog.com/en/media-center/cad-libraries](http://www.camlog.com/en/media-center/cad-libraries)

Medentika® and Preface® are registered trademarks of Medentika GmbH, D-Hügelsheim.



## Accessories for CAM titanium blanks, type IAC

	Article	Art. No.	Ø
	<b>CONELOG® Collet for CAM blank, type IAC*</b> Ø 6 mm, length 17 mm, incl. 2 fixing screws for CAM blank, type IAC  <b>Material</b> Stainless steel	C3720.3300	3.3 mm
		C3720.4300	3.8 mm
			4.3 mm
		C3720.5000	5.0 mm



\* Type IAC

For the milling process, the CAM titanium blank, type IAC is fixated to the implant-abutment connection via the CONELOG® Collet for CAM blanks. The machine-specific holders and adapters for the collet as well as the milling strategies are to be provided by the user.



# Esthomic® Abutments

## Cemented crown and bridge restorations


	Article	Art. No.	Ø	GH
	<b>CONOLOG® Esthomic® Abutments, straight</b> preparable, incl. abutment screw  <b>Material</b> Titanium alloy	C2226.3815	3.8 mm	1.5–2.5 mm
		C2226.3830		3.0–4.5 mm
		C2226.4315	4.3 mm	1.5–2.5 mm
		C2226.4330		3.0–4.5 mm
		C2226.5015	5.0 mm	1.5–2.5 mm
		C2226.5030		3.0–4.5 mm
	<b>CONOLOG® Esthomic® Abutments, Inset</b> preparable, incl. abutment screw  <b>Material</b> Titanium alloy	C2235.3320*	3.3 mm	2.0–3.3 mm
		C2235.3820	3.8 mm	
		C2235.4320	4.3 mm	
		C2235.5020	5.0 mm	

\* only for crown restorations in the region of the upper lateral and lower lateral and central incisors

	Article	Art. No.	Ø	GH
	<b>CONELOG® Esthomic® Abutments 15° angled, type A</b> preparable, incl. abutment screw  <b>Material</b> Titanium alloy	C2227.3815	3.8 mm	1.5–2.5 mm
		C2227.3830		3.0–4.5 mm
		C2227.4315	4.3 mm	1.5–2.5 mm
		C2227.4330		3.0–4.5 mm
		C2227.5015	5.0 mm	1.5–2.5 mm
		C2227.5030		3.0–4.5 mm
	<b>CONELOG® Esthomic® Abutments 15° angled, type B</b> preparable, incl. abutment screw  <b>Material</b> Titanium alloy	C2228.3815	3.8 mm	1.5–2.5 mm
		C2228.3830		3.0–4.5 mm
		C2228.4315	4.3 mm	1.5–2.5 mm
		C2228.4330		3.0–4.5 mm
		C2228.5015	5.0 mm	1.5–2.5 mm
		C2228.5030		3.0–4.5 mm
	<b>CONELOG® Esthomic® Abutments 20° angled, type A</b> preparable, incl. abutment screw  <b>Material</b> Titanium alloy	C2231.3815	3.8 mm	1.5–2.5 mm
		C2231.3830		3.0–4.5 mm
		C2231.4315	4.3 mm	1.5–2.5 mm
		C2231.4330		3.0–4.5 mm
		C2231.5015	5.0 mm	1.5–2.5 mm
		C2231.5030		3.0–4.5 mm
	<b>CONELOG® Esthomic® Abutments 20° angled, type B</b> preparable, incl. abutment screw  <b>Material</b> Titanium alloy	C2232.3815	3.8 mm	1.5–2.5 mm
		C2232.3830		3.0–4.5 mm
		C2232.4315	4.3 mm	1.5–2.5 mm
		C2232.4330		3.0–4.5 mm
		C2232.5015	5.0 mm	1.5–2.5 mm
		C2232.5030		3.0–4.5 mm


## Universal abutments

### Cemented crown and bridge restoration

	Article	Art. No.	Ø	Dimension
 <p>11 mm</p>	<b>CONELOG® Universal abutment</b> preparable, incl. abutment screw  <b>Material</b> Titanium alloy	C2211.3300*	3.3 mm	
		C2211.3800	3.8 mm	
		C2211.4300	4.3 mm	
		C2211.5000	5.0 mm	




## Gold-plastic abutment

### Cemented crown and bridge restoration

	Article	Art. No.	Ø	Noble metal weight
 <p>11.7 mm</p>	<b>CONELOG® Gold-plastic abutment</b> cast-on, incl. abutment screw  <b>Material</b> Cast-on gold alloy / POM	C2246.3300*	3.3 mm	approx. 0.31 g
		C2246.3800	3.8 mm	approx. 0.36 g
		C2246.4300	4.3 mm	approx. 0.36 g
		C2246.5000	5.0 mm	approx. 0.55 g











\* only for crown restorations in the region of the upper lateral and lower lateral and central incisors  
 (Ø 3.3 mm not for double crown restorations)





## Occlusally screw-mounted prosthetics

	Article	Art. No.	Type	Ø	GH	PP Ø			
	<b>CONELOG®</b> <b>Bar abutments, straight</b> sterile  <b>Material</b> Titanium alloy	C2254.3310	-	3.3 mm	1.0 mm	4.3 mm			
		C2254.3325			2.5 mm				
		C2254.3810		3.8 mm	1.0 mm		4.3 mm		
		C2254.3825			2.5 mm				
		C2254.3840		4.0 mm					
		C2254.4310		4.3 mm	1.0 mm			4.3 mm	
		C2254.4325			2.5 mm				
		C2254.4340		4.0 mm					
		C2254.5010		5.0 mm	1.0 mm	6.0 mm			
		C2254.5025			2.5 mm				
C2254.5040	4.0 mm								
	<b>CONELOG®</b> <b>Bar abutments, 17° angled</b> incl. light blue anodized abutment screw with reduced head, sterile  <b>Material</b> Titanium alloy	C2256.3325	A	3.3 mm	2.5 mm	4.3 mm			
		C2256.3340			4.0 mm				
		C2257.3325	B		2.5 mm		4.3 mm		
		C2257.3340			4.0 mm				
		C2256.3825	A		3.8 mm			2.5 mm	4.3 mm
		C2256.3840						4.0 mm	
		C2257.3825	B	2.5 mm	4.3 mm				
		C2257.3840		4.0 mm					
		C2256.4325	A	4.3 mm		2.5 mm	4.3 mm		
		C2256.4340				4.0 mm			
		C2257.4325	B			2.5 mm		4.3 mm	
		C2257.4340				4.0 mm			
		C2256.5025	A		5.0 mm	2.5 mm			6.0 mm
		C2256.5040				4.0 mm			
C2257.5025	B	2.5 mm	6.0 mm						
C2257.5040		4.0 mm							
	<b>CONELOG®</b> <b>Bar abutments, 30° angled</b> incl. light blue anodized abutment screw with reduced head, sterile  <b>Material</b> Titanium alloy	C2258.3325		A		3.3 mm	2.5 mm	4.3 mm	
		C2258.3340					4.0 mm		
		C2259.3325		B	2.5 mm		4.3 mm		
		C2259.3340			4.0 mm				
		C2258.3825	A	3.8 mm	2.5 mm				4.3 mm
		C2258.3840			4.0 mm				
		C2259.3825	B	2.5 mm	4.3 mm				
		C2259.3840		4.0 mm					
		C2258.4325	A	4.3 mm		2.5 mm	4.3 mm		
		C2258.4340				4.0 mm			
		C2259.4325	B			2.5 mm		4.3 mm	
		C2259.4340				4.0 mm			
		C2258.5035	A		5.0 mm	3.5 mm			6.0 mm
		C2258.5050				5.0 mm			
		C2259.5035	B	3.5 mm		6.0 mm			
		C2259.5050		5.0 mm					






Types A and B see page 8

Occlusally screw-mounted prosthetics

	Article	Art. No.	Ø			Dimensionen
	<b>Orientation gauge for COMFOUR®</b> for Ø 2.0 mm pilot drilling  <b>Material</b> Nitinol	J3551.0001	-			-
	<b>Aligning tool</b> for angled bar abutments, for insertion posts	J2269.0005	-			17°
	<b>Material</b> Stainless steel	J2269.0006	-			30°
	<b>Gingiva height indicator, straight</b>  <b>Material</b> Titanium alloy	J3550.3300	3.3 mm			-
		J3550.3800	3.8 mm			
		J3550.4300	4.3 mm			
		J3550.5000	5.0 mm			
	<b>Insertion tool for impression posts and healing caps for bar abutments</b>  <b>Material</b> Stainless steel	J5300.0027	3.3 mm	3.8 mm	4.3 mm	19.1 mm
		J5300.0028	5.0 mm			
	<b>Healing cap for bar abutment</b> light blue partially anodized, sterile  <b>Material</b> Titanium alloy	J2029.4300	3.3 mm	3.8 mm	4.3 mm	-
		J2029.6000	5.0 mm			
	<b>Impression cap, short, for bar abutment, closed tray (bridge/bar)</b> light blue partially anodized, sterile  <b>Material</b> Titanium alloy	J2129.4300	3.3 mm	3.8 mm	4.3 mm	6.5 mm
		J2129.6000	5.0 mm			7.0 mm
	<b>Impression cap, long, for bar abutment, closed tray (bridge/bar)</b> light blue partially anodized, sterile  <b>Material</b> Titanium alloy	J2129.4310	3.3 mm	3.8 mm	4.3 mm	11.0 mm
		J2129.6010	5.0 mm			
	<b>Bar lab analog for bar abutments</b>  <b>Material</b> Stainless steel	J3020.4300	3.3 mm	3.8 mm	4.3 mm	-
		J3020.6000	5.0 mm			
	<b>Bar implant analog for bar abutments</b> for printed and cast models  <b>Material</b> Stainless steel	J3025.4300	3.3 mm	3.8 mm	4.3 mm	-
		J3025.6000	5.0 mm			
	<b>Scanning cap for bar abutments</b> incl. prosthetic screw, light blue anodized, sterile  <b>Material</b> PEEK	J2610.4300	3.3 mm	3.8 mm	4.3 mm	-
		J2610.6000	5.0 mm			


	Article	Art. No.	Ø			Dimensions
	<b>Titanium cap for bar abutment, for crown</b> incl. prosthetic screw, light blue anodized, sterile	J2259.4301	3.3 mm	3.8 mm	4.3 mm	-
	<b>Material</b> Titanium alloy	J2259.6001	5.0 mm			
	<b>Titanium cap for bar abutment, for bridge</b> incl. prosthetic screw, light blue anodized, sterile	J2259.4302	3.3 mm	3.8 mm	4.3 mm	-
	<b>Material</b> Titanium alloy	J2259.6002	5.0 mm			
	<b>Titanium cap without retention for bar abutment, for bridge</b> incl. prosthetic screw, light blue anodized	J2259.4322	3.3 mm	3.8 mm	4.3 mm	-
	<b>Material</b> Titanium alloy	J2259.6022	5.0 mm			
	<b>Crown base for bar abutment</b> burn-out	J2256.4306	3.3 mm	3.8 mm	4.3 mm	-
	<b>Material</b> POM	J2256.6006	5.0 mm			
	<b>Base for bar abutment</b> burn-out	J2257.4301	3.3 mm	3.8 mm	4.3 mm	-
	<b>Material</b> POM	J2257.6001	5.0 mm			
	<b>Base for bar abutment</b> cast-on	J2263.4300	3.3 mm	3.8 mm	4.3 mm	approx. 0.48 g
	<b>Material</b> Cast-on gold alloy / POM	J2263.6000	5.0 mm			approx. 0.70 g
	<b>Base for bar abutment</b> solderable	J2258.4300	3.3 mm	3.8 mm	4.3 mm	-
	<b>Material</b> Solderable gold alloy	J2258.6000	5.0 mm			
	<b>Base for bar abutment, titanium</b> laser-weldable	J2262.4300	3.3 mm	3.8 mm	4.3 mm	-
	<b>Material</b> Titanium Grade 4	J2262.6000	5.0 mm			
	<b>Titanium bonding base for bar abutment</b> Passive Fit	J2260.4301	3.3 mm	3.8 mm	4.3 mm	-
	<b>Material</b> Titanium alloy	J2260.6001	5.0 mm			
	<b>Bar sleeve for titanium bonding base</b> burn-out, Passive-Fit, incl. prosthetic screw for bar abutment, hex, (only for fabrication of the cast framework in conjunction with bar sleeves for titanium bonding base Passive Fit)	J2261.4301	3.3 mm	3.8 mm	4.3 mm	-
	<b>Material</b> POM	J2261.6001	5.0 mm			

Occlusally screw-mounted prosthetics

	Article	Art. No.	Ø			Thread
	<b>Polishing protection for caps and bases for bar abutment</b>	J3021.4300	3.3 mm	3.8 mm	4.3 mm	M1.6
	<b>Material</b> Titanium alloy	J3021.6000	5.0 mm			M2.0
	<b>CONELOG® Abutment screw</b> with reduced head, hex, light blue anodized	C4004.1601	3.3 mm	3.8 mm	4.3 mm	M1.6
	<b>Material</b> Titanium alloy	C4004.2001	5.0 mm			M2.0
	<b>CONELOG® Lab screw</b> with reduced head, hex, light blue partially anodized	C4004.1600	3.3 mm	3.8 mm	4.3 mm	M1.6
	<b>Material</b> Titanium alloy	C4004.2000	5.0 mm			M2.0
	<b>Prosthetic screw for bar abutment</b> hex, light blue anodized (for final fixation of the restoration)	J4012.1601	3.3 mm	3.8 mm	4.3 mm	M1.6
	<b>Material</b> Titanium alloy	J4012.2001	5.0 mm			M2.0
	<b>Lab prosthetic screw for bar abutment</b> hex, brown anodized	J4013.1601	3.3 mm	3.8 mm	4.3 mm	M1.6
	<b>Material</b> Titanium alloy	J4013.2001	5.0 mm			M2.0

Lab screws must not be used on patients!



	Article	Art. No.	Ø	Thread
	<b>Screw, hex, length 10 mm</b> can be shortened by 2.5 mm, light blue anodized, sterile	J4012.1610	-	M1.6
	<b>Material</b> Titanium alloy	J4012.2010		M2.0
	<b>Screw, hex, length 15 mm</b> can be shortened by 2.5 mm, light blue anodized, sterile	J4012.1615	-	M1.6
	<b>Material</b> Titanium alloy	J4012.2015		M2.0
	<b>Screw, hex, length 20 mm</b> can be shortened by 2.5 mm, light blue anodized, sterile	J4012.1620	-	M1.6
	<b>Material</b> Titanium alloy	J4012.2020		M2.0
	<b>Plastic screw for bar abutment</b> Hex, length 27 mm, sterile	J4009.1627	-	M1.6
	<b>Material</b> PEEK	J4009.2027		M2.0



# We are Implantology





**Combined forces. Accelerated evolution.**

**Inspired to achieve excellence in oral reconstruction, we use our combined forces to accelerate evolution within global implantology.**

Since 2016, BioHorizons and Camlog have been strategically joining forces under the umbrella of the Henry Schein Global Oral Reconstruction Group.

[www.biohorizonscamlog.com](http://www.biohorizonscamlog.com)





# Ball abutment anchoring system


	Article	Art. No.	Ø	GH
	<b>CONELOG® Ball abutment, male part</b> incl. stabilizing ring  <b>Material</b> Titanium alloy / plastic	C2249.3315	3.3 mm	1.5 mm
		C2249.3330		3.0 mm
		C2249.3815	3.8 mm	1.5 mm
		C2249.3830		3.0 mm
		C2249.3845	4.5 mm	
		C2249.4315	4.3 mm	1.5 mm
		C2249.4330		3.0 mm
		C2249.4345		4.5 mm
		C2249.5015	5.0 mm	1.5 mm
		C2249.5030		3.0 mm
C2249.5045	4.5 mm			
	<b>CM Dalbo®-Plus matrix</b> for ball abutment, incl. lamella retention insert and duplicating aid  <b>Material</b> Titanium Grade 4 / gold alloy	05003503	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	
	<b>Lamella retention insert</b> for CM Dalbo®-Plus matrix  <b>Material</b> Gold alloy	05003504	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	
	<b>Ball abutment analog</b> incl. stabilizing ring  <b>Material</b> Brass/plastic	C3015.3300	3.3 mm	-
			3.8 mm	
			4.3 mm	
		C3015.5000	5.0 mm	

Dalbo®-Plus is a registered trademark of Cendres + Métaux SA, Bienne, Switzerland.

# Locator® Anchoring System




## CONELOG® Locator R-Tx®





	Article	Art. No.	Ø	GH
	<b>CONELOG® Locator R-Tx® Abutment</b> incl. retention housing with black processing replacement male, block out spacer white and four different replacement males  <b>Material</b> Titanium alloy / Nylon	30805-01	3.3 mm	1.0 mm
		30805-02		2.0 mm
		30805-03		3.0 mm
		30805-04		4.0 mm
		30806-01	3.8 mm	1.0 mm
		30806-02		2.0 mm
		30806-03		3.0 mm
		30806-04		4.0 mm
		30806-05	4.3 mm	5.0 mm
		30807-01		1.0 mm
		30807-02		2.0 mm
		30807-03		3.0 mm
		30807-04	5.0 mm	4.0 mm
		30807-05		5.0 mm
		30808-01		1.0 mm
		30808-02		2.0 mm
		30808-03	5.0 mm	3.0 mm
		30808-04		4.0 mm
30808-05	5.0 mm			
	<b>Locator R-Tx® Impression cap</b> (4 units)  <b>Material</b> Polyethylene	30017-01	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	
	<b>Locator R-Tx® Analog</b> Ø 3.35 mm (4 units)  <b>Material</b> Aluminum	30014-01	3.3 mm	-
			3.8 mm	
			4.3 mm	
	<b>Locator R-Tx® Analog</b> Ø 5.0 mm (4 units)  <b>Material</b> Aluminum	30016-01	5.0 mm	-

	Article	Art. No.	Ø
	<b>Locator R-Tx® Retention housing</b> with processing replacement male, black (4 units)  <b>Material</b> Titanium alloy / polyethylene	30013-01	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	<b>Locator R-Tx® Processing replacement male</b> black (4 units)  <b>Material</b> Polyethylene	30012-01	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	<b>Locator R-Tx® Spacer/duplication aid</b> (4 units)  <b>Material</b> Polyethylene	30018-01	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	<b>Locator R-Tx® Replacement male</b> gray, NO RETENTION (4 units)  <b>Material</b> Nylon	30001-01	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	<b>Locator R-Tx® Replacement male</b> blue, LOW (4 units)  <b>Material</b> Nylon	30002-01	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	<b>Locator R-Tx® Replacement male</b> pink, MEDIUM (4 units)  <b>Material</b> Nylon	30003-01	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	<b>Locator R-Tx® Replacement male</b> white, HIGH (4 units)  <b>Material</b> Nylon	30004-01	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm

# Locator® Anchoring System





## CONELOG® Locator®

	Article	Art. No.	Ø	GH
	<b>CONELOG® Locator® Abutment</b>  <b>Material</b> Titanium alloy / TiN	C2253.3310	3.3 mm	1.0 mm
		C2253.3320		2.0 mm
		C2253.3330		3.0 mm
		C2253.3340		4.0 mm
		C2253.3810	3.8 mm	1.0 mm
		C2253.3820		2.0 mm
		C2253.3830		3.0 mm
		C2253.3840		4.0 mm
		C2253.3850		5.0 mm
		C2253.4310	4.3 mm	1.0 mm
		C2253.4320		2.0 mm
		C2253.4330		3.0 mm
		C2253.4340		4.0 mm
		C2253.4350	5.0 mm	
		C2253.5010	5.0 mm	1.0 mm
		C2253.5020		2.0 mm
		C2253.5030		3.0 mm
C2253.5040	4.0 mm			
C2253.5050	5.0 mm			
	<b>Locator® Impression cap</b> (4 units)  <b>Material</b> Aluminum/polyethylene	J2253.0200	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	
	<b>Locator® Analog</b> (4 units)  <b>Material</b> Aluminum	J2253.0340	3.3 mm	-
			3.8 mm	
			4.3 mm	
			5.0 mm	

	Article	Art. No.	Ø
	<b>Locator® Lab kits</b> (2 units)  <b>Contents per kit:</b> 1 Retention housing with processing replacement male 1 Block out spacer, white 1 Replacement male, clear 1 Replacement male, pink 1 Replacement male, blue  <b>Material</b> Titanium alloy / polyethylene / Teflon / Nylon	J2253.0102	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	<b>Locator® Lab kits for extended angulation</b> (2 units)  <b>Contents per kit:</b> 1 Retention housing with processing replacement male 1 Block out spacer, white 1 Replacement male, green 1 Replacement male, orange 1 Replacement male, red  <b>Material</b> Titanium alloy / polyethylene / Teflon / Nylon	J2253.0112	3.8 mm
			4.3 mm
			5.0 mm
	<b>Locator® Block out spacer</b> (20 units)  <b>Material</b> Teflon	J2253.0401	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	<b>Locator® Processing replacement male</b> (4 units)  <b>Material</b> Polyethylene	J2253.0402	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm

# Locator® Anchoring System

## CONELOG® Locator®



	Article	Art. No.	Ø
	<b>Locator® Replacement male</b> clear, HIGH, Div.: 0°-10° (4 units)  <b>Material</b> Nylon	J2253.1005	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	<b>Locator® Replacement male</b> pink, MEDIUM, Div.: 0°-10° (4 units)  <b>Material</b> Nylon	J2253.1003	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	<b>Locator® Replacement male</b> blue, LOW, Div.: 0°-10° (4 units)  <b>Material</b> Nylon	J2253.1002	3.3 mm
			3.8 mm
			4.3 mm
			5.0 mm
	<b>Locator® Replacement male for extended angulation</b> green, HIGH, Div.: 10°-20° (4 units)  <b>Material</b> Nylon	J2253.2004*	3.8 mm
			4.3 mm
			5.0 mm
	<b>Locator® Replacement male for extended angulation</b> orange, MEDIUM, Div.: 10°-20° (4 units)  <b>Material</b> Nylon	J2253.2003*	3.8 mm
			4.3 mm
			5.0 mm
	<b>Locator® Replacement male for extended angulation</b> red, LOW, Div.: 10°-20° (4 units)  <b>Material</b> Nylon	J2253.2002*	3.8 mm
			4.3 mm
			5.0 mm
	<b>Locator® Replacement male for extended angulation</b> gray, NO RETENTION, Div.: 0°-20° (4 units)  <b>Material</b> Nylon	J2253.2000*	3.8 mm
			4.3 mm
			5.0 mm

\* not permitted for implant Ø 3.3 mm




Manufacturer Locator®: Zest Anchors | 2875 Loker Avenue East, Carlsbad | California 92010 | USA  
Locator® and Locator R-Tx® are registered trademarks of the Zest Anchors company.



## Double crown restoration

	Article	Art. No.	Ø
 11 mm	<b>CONELOG® Universal abutment for the double crown technique</b> preparable, incl. CONELOG® Abutment screw  <b>Material</b> Titanium alloy	C2211.3800	3.8 mm
		C2211.4300	4.3 mm
		C2211.5000	5.0 mm
 12 mm	<b>CONELOG® Telescope abutment for the double crown technique</b> preparable, incl. CONELOG® Abutment screw  <b>Material</b> Titanium alloy	C2212.3800	3.8 mm
		C2212.4300	4.3 mm
		C2212.5000	5.0 mm

## Accessories for abutments



	Article	Art. No.	Ø	Thread
	<b>CONELOG® Abutment screw, hex</b> for the final screwing of abutments into the implant  <b>Material</b> Titanium alloy	C4005.1601	3.3 mm	M1.6
			3.8 mm	
			4.3 mm	
		C4005.2001	5.0 mm	M2.0
	<b>CONELOG® Lab screw, hex</b> for fixation on the working model, brown anodized  <b>Material</b> Titanium alloy	C4006.1601	3.3 mm	M1.6
			3.8 mm	
			4.3 mm	
		C4006.2001	5.0 mm	M2.0
	<b>CONELOG® Lab screw, hex (3 units)</b> for fixation on the working model, brown anodized  <b>Material</b> Titanium alloy	C4006.1603	3.3 mm	M1.6
			3.8 mm	
			4.3 mm	
		C4006.2003	5.0 mm	M2.0

"CONELOG® Abutment Screw for CONELOG® Titanium Base CAD/CAM dark purple anodized" must be used for titanium bases, (see page 69).


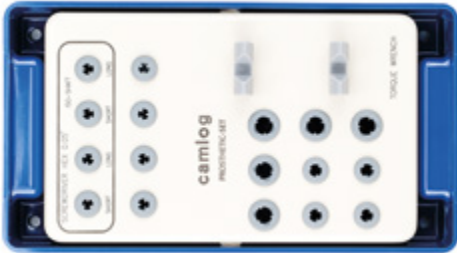




**Lab screws must not be used on patients!**




## Prosthetic instruments



	Article	Art. No.	L
	<p><b>Torque wrench</b> with continuous torque adjustment until maximal 30 Ncm</p> <p><b>Material</b> Stainless steel</p>	J5320.1030	-
	<p><b>Insertion tool</b> for ball abutment, manual/wrench</p> <p><b>Material</b> Stainless steel</p>	J5300.0011	18.3 mm
	<p><b>Screwdriver activator</b> for CM Dalbo®-Plus ball abutment matrix</p> <p><b>Material</b> Stainless steel</p>	07000389	-
	<p><b>Insertion tool for straight bar abutments, short</b> Ø 3.3/3.8/4.3 mm</p> <p><b>Material</b> Stainless steel</p>	J5300.0020	18.6 mm
	<p><b>Insertion tool for straight bar abutments, short</b> Ø 5.0 mm</p> <p><b>Material</b> Stainless steel</p>	J5300.0025	18.6 mm

	Article	Art. No.	L
	<p><b>Insertion tool for straight bar abutments, long</b> Ø 3.3/3.8/4.3 mm</p> <p><b>Material</b> Stainless steel</p>	J5300.0021	28.0 mm
	<p><b>Insertion tool for impression posts and healing caps for bar abutments</b> Ø 3.3/3.8/4.3 mm</p> <p><b>Material</b> Stainless steel</p>	J5300.0027	19.1 mm
	<p><b>Insertion tool for impression posts and healing caps for bar abutments</b> Ø 5.0 mm</p> <p><b>Material</b> Stainless steel</p>	J5300.0028	19.1 mm
	<p><b>Insertion tool</b> for Locator®, manual/wrench</p> <p><b>Material</b> Stainless steel</p>	J2253.0001	24.3 mm
	<p><b>Locator® Instrument</b> 3-part</p> <p><b>Material</b> Stainless steel</p>	J2253.0002	83.0 mm
	<p><b>Locator® Abutment holder sleeve</b> for golden element of the Locator® Instrument (4 units)</p> <p><b>Material</b> Polysulfone</p>	08394	-
	<p><b>Locator® Angle measurement guide</b></p> <p><b>Material</b> Stainless steel</p>	J2253.0003	-
	<p><b>Locator® Parallel post</b> (4 units)</p> <p><b>Material</b> Polyethylene</p>	J2253.0004	-






## Prosthetic instruments

	Article	Art. No.	Dimensions
	<p><b>Locator R-Tx®</b> Insertion tool for replacement males with plastic handle</p> <p><b>Material</b> Stainless steel</p>	30021-01	-
	<p><b>Prosthetic tray</b> (without content)</p> <p><b>Material</b> Plastic</p>	J5330.8500	197 × 108 × 54 mm
	<p><b>Prosthetic tray Universal</b> (without content) resterilizable</p> <p><b>Material</b> Radel®, silicone</p>	J5330.8700	162 × 73 × 29 mm
	<p><b>Screwdriver</b> hex, extra short, manual/wrench</p> <p><b>Material</b> Stainless steel</p>	J5317.0510	14.5 mm
	<p><b>Screwdriver</b> hex, short, manual/wrench</p> <p><b>Material</b> Stainless steel</p>	J5317.0501	22.5 mm
	<p><b>Screwdriver</b> hex, long, manual/wrench</p> <p><b>Material</b> Stainless steel</p>	J5317.0502	30.3 mm

	Article	Art. No.	L
	<b>Screwdriver</b> hex, short, ISO shaft  <b>Material</b> Stainless steel	J5317.0504	18.0 mm
	<b>Screwdriver</b> hex, long, ISO shaft  <b>Material</b> Stainless steel	J5317.0503	26.0 mm
	<b>Manual screwdriver</b> hex, without wrench head connection  <b>Material</b> Stainless steel	J5317.0511	23.0 mm

	Article	Art. No.	Ø	Thread
	<b>CONELOG® Disconnectors</b> for CONELOG® Abutments, short  <b>Material</b> Stainless steel	C5300.1601	3.3 mm	M1.6
			3.8 mm	
			4.3 mm	
		C5300.2001	5.0 mm	M2.0
	<b>CONELOG® Disconnectors</b> for CONELOG® Abutments, long  <b>Material</b> Stainless steel	C5300.1603	3.3 mm	M1.6
			3.8 mm	
			4.3 mm	
		C5300.2003	5.0 mm	M2.0

## Instruments for dental technicians

	Article	Art. No.	Ø
	<b>Handle for CAMLOG®/CONOLOG® Implant analog</b>  <b>Material</b> Stainless steel	J3025.0010	3.3 mm
			3.8 mm
			4.3 mm
		J3025.0015	5.0 mm
	<b>Universal holder</b> incl. 2 CONELOG® Lab screws, hex, and 1 each CONELOG® Abutment collet Ø 3.3/3.8/4.3/5.0 mm  <b>Material</b> Stainless steel / titanium alloy	C3709.0010	-
	<b>Universal holder</b>  <b>Material</b> Stainless steel	J3709.0015	-
	<b>CONELOG® Abutment collet</b> for universal holder, for grinding CONELOG® Abutments  <b>Material</b> Titanium alloy	C3709.3300	3.3 mm
		C3709.3800	3.8 mm
		C3709.4300	4.3 mm
		C3709.5000	5.0 mm
	<b>Reworking reamer, base for bar abutment</b> plane surface/cone seat, for burn-out caps  <b>Material</b> Stainless steel / brass	J3711.0010	3.3 mm
			3.8 mm
			4.3 mm
		J3711.0015	5.0 mm
	<b>Reworking reamer, base for bar abutment</b> screw seat, for burn-out caps  <b>Material</b> Stainless steel / brass	J3711.0020	3.3 mm
			3.8 mm
			4.3 mm
		J3711.0025	5.0 mm

# Selection Abutments

	Article	Art. No.
	<b>CONELOG® Selection abutment kit</b> (Contents: 2 units each, according to table below)	C8011.1000

Contents: CONELOG® Selection abutment kit					
Article	Material	Ø			GH
CONELOG® Esthomic® Selection abutment , straight*	POM	3.8 mm	4.3 mm	1.5-2.5	3.0-4.5
CONELOG® Esthomic® Selection abutment, 15° angled, type A*				1.5-2.5	
CONELOG® Esthomic® Selection abutment, 15° angled, type B*				1.5-2.5	
CONELOG® Esthomic® Selection abutment, 20° angled, type A*				1.5-2.5	
CONELOG® Esthomic® Selection abutment, 20° angled, type B*				1.5-2.5	

\* These products are not available singly.

**Selection abutments must not be used on patients!**





# Auxiliary Articles








## Implants for practice

	Article	Art. No.	Ø	L
	<b>CONELOG® PROGRESSIVE-LINE Implant for practice</b> incl. snap-in insertion post and cover screw, brown anodized  <b>Material</b> Titanium alloy	C1901.3813	3.8 mm	13 mm
	<b>CONELOG® PROGRESSIVE-LINE Implant for practice</b> incl. snap-in insertion post and cover screw, brown anodized  <b>Material</b> Titanium alloy	C1901.4313	4.3 mm	
	<b>CONELOG® SCREW-LINE Implant for practice</b> incl. insertion post and cover screw, brown anodized  <b>Material</b> Titanium alloy	C1069.3813	3.8 mm	13 mm
	<b>CONELOG® SCREW-LINE Implant for practice</b> incl. insertion post and cover screw, brown anodized  <b>Material</b> Titanium alloy	C1069.4313	4.3 mm	

Implants for practice must not be used on patients!



## Insertion posts

	Article	Art. No.	Ø
	<b>CONELOG® Insertion post, screw-mounted</b> for CONELOG® Lab analog/implant analog, incl. fixing screw (2 units)  <b>Material</b> Titanium alloy	C2026.3303	3.3 mm
		C2026.3803	3.8 mm
		C2026.4303	4.3 mm
		C2026.5003	5.0 mm

## Demonstration models




	Article	Art. No.
	<p><b>CONELOG® Demonstration model, acrylic glass</b> Upper jaw, 4 CONELOG® SCREW-LINE Implants, 4 × Ø 4.3 mm</p> <p><b>Material</b> Acrylic glass / titanium</p>	C8070.1020
	<p><b>CONELOG® Demonstration model, acrylic glass</b> Lower jaw, 4 CONELOG® SCREW-LINE Implants, 4 × Ø 4.3 mm</p> <p><b>Material</b> Acrylic glass / titanium</p>	C8050.1040
	<p><b>Edentulous mandible</b> incl. mounting plate</p> <p><b>Material</b> Plastic</p>	J8070.2050

## Macro Models




	Article	Art. No.
	<p><b>CONELOG® PROGRESSIVE-LINE Macro model</b> Scale 3:1</p> <p><b>Content:</b> 1 CONELOG® PROGRESSIVE-LINE Implant 1 CONELOG® Esthomic® Abutment , straight 1 CONELOG® Abutment screw, hex 1 CONELOG® Screwdriver, hex 1 Premolar, suitable for CONELOG® Esthomic® Abutment, straight 1 Acrylic base</p> <p><b>Material</b> Plastic / stainless steel</p>	C8010.1400
	<p><b>CONELOG® SCREW-LINE Macro model</b> Scale 3:1</p> <p><b>Content:</b> 1 CONELOG® SCREW-LINE Implant 1 CONELOG® Esthomic® Abutment , straight 1 CONELOG® Abutment screw, hex 1 Screwdriver, hex 1 Premolar, suitable for CONELOG® Esthomic® Abutment, straight 1 Acrylic base</p> <p><b>Material</b> Plastic / stainless steel</p>	C8010.1010

# Literature

	Article	Media No. / Art. No.
	<p><b>Patient brochure</b> Dental implants – inspired by nature</p>	<p>M-0431-BRO-EN-INT- BHCL-00-052023</p>
	<p><b>COMFOUR® Patient brochure</b> Bridge instead of dentures – dental prosthesis with feel-good factor</p>	<p>M-1437-BRO-EN-INT- BHCL-00-052023</p>
	<p><b>Biomaterial patient brochure</b> Stable bone and a firm gingiva – the basis of oral health</p>	<p>M-0151-BRO-EN-INT- BHCL-00-052023</p>
	<p><b>Patient Documentation and Implant Card</b> Patient-specific documentation of implant restoration</p>	<p>J8000.0372</p>
	<p><b>Patient advice sheets</b> Set, A4</p>	<p>M-0584-FLY-EN-INT- BHCL-00-052023</p>

	Article	Media No.
	<p><b>Presentation folder</b> A4, laminated</p>	<p>M-0258-BUE-EN-INT- BHCL-00-052023</p>
	<p><b>Poster</b> Dental implants – inspired by nature Format: 50 × 70 cm</p>	<p>M-1628-PST-EN-INT- BHCL-00-052023</p>
	<p><b>Appointment pad</b> 50 sheets/pad, A7 Packaging units: 5 units</p>	<p>M-1629-FOR-EN-INT- BHCL-052023</p>

# Literature












	Article	Media No. / Art. No.
	<p><b>Patient flyer</b> Single tooth</p>	<p>M-0446-FLY-EN-INT- BHCL-00-072021</p>
	<p><b>Patient flyer</b> Multiple teeth solution</p>	<p>M-0447-FLY-EN-INT- BHCL-00-072021</p>
	<p><b>Patient flyer</b> Edentulous</p>	<p>M-0448-FLY-EN-INT- BHCL-00-072021</p>













[www.biohorizonscamlog.com/patient-information](http://www.biohorizonscamlog.com/patient-information)



# Indication overview

Single-tooth restoration		Bridge re
Cemented	Screw-mounted	Cemented
	 <p>Temporary abutments, titanium alloy, crown</p>	
 <p>Esthomic® Abutments</p>		 <p>Esthomic® Abutments</p>
	 <p>Bar abutments</p>	
 <p>Titanium base CAD/CAM, crown</p>	 <p>Titanium base CAD/CAM, crown</p>	 <p>Titanium base CAD/CAM, bridge</p>
 <p>Universal abutment      CAM blank</p>		 <p>Universal abutment      CAM blank</p>
 <p>Gold-plastic abutment</p>	 <p>Gold-plastic abutment</p>	 <p>Gold-plastic abutment</p>





Restoration	Hybrid restoration
Screw-mounted	Removable (full denture)
 <p>Temporary abutments, titanium alloy, bridge</p>	
 <p>Bar abutments</p>	 <p>Bar abutments</p>
 <p>Titanium base CAD/CAM, bridge</p>	
	 <p>Locator® Anchoring System</p>
	 <p>Ball abutment</p>
	 <p>Universal abutment      CAM blank</p>
	 <p>Telescope abutment</p>
	 <p>Gold-plastic abutment</p>
	 <p>Titanium base CAD/CAM, crown</p>


Double crown restoration

Additional Information



# Implant overview

## PROGRESSIVE-LINE

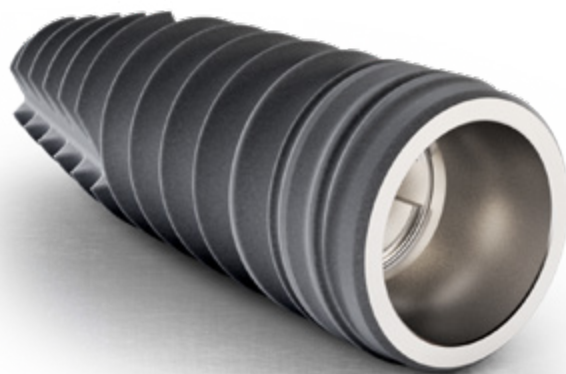	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article	Art. No. A Ø				L
 <p><b>CONELOG® PROGRESSIVE-LINE Implant, Promote® plus</b> with snap-in insertion post</p>	-	C1086.3807 A Ø 3.0 mm	C1086.4307 A Ø 3.0 mm	C1086.5007 A Ø 3.5 mm	7 mm
	C1086.3309 A Ø 2.2 mm	C1086.3809 A Ø 3.0 mm	C1086.4309 A Ø 3.0 mm	C1086.5009 A Ø 3.5 mm	9 mm
	C1086.3311 A Ø 2.2 mm	C1086.3811 A Ø 2.7 mm	C1086.4311 A Ø 2.7 mm	C1086.5011 A Ø 3.2 mm	11 mm
	C1086.3313 A Ø 2.2 mm	C1086.3813 A Ø 2.7 mm	C1086.4313 A Ø 2.7 mm	C1086.5013 A Ø 3.2 mm	13 mm
	C1086.3316 A Ø 2.2 mm	C1086.3816 A Ø 2.7 mm	C1086.4316 A Ø 2.7 mm	C1086.5016 A Ø 3.2 mm	16 mm
 <p><b>CONELOG® PROGRESSIVE-LINE Implant, Promote® plus</b> with screw-mounted insertion post</p>	-	C1085.3807 A Ø 3.0 mm	C1085.4307 A Ø 3.0 mm	C1085.5007 A Ø 3.5 mm	7 mm
	C1085.3309 A Ø 2.2 mm	C1085.3809 A Ø 3.0 mm	C1085.4309 A Ø 3.0 mm	C1085.5009 A Ø 3.5 mm	9 mm
	C1085.3311 A Ø 2.2 mm	C1085.3811 A Ø 2.7 mm	C1085.4311 A Ø 2.7 mm	C1085.5011 A Ø 3.2 mm	11 mm
	C1085.3313 A Ø 2.2 mm	C1085.3813 A Ø 2.7 mm	C1085.4313 A Ø 2.7 mm	C1085.5013 A Ø 3.2 mm	13 mm
	C1085.3316 A Ø 2.2 mm	C1085.3816 A Ø 2.7 mm	C1085.4316 A Ø 2.7 mm	C1085.5016 A Ø 3.2 mm	16 mm





## SCREW-LINE

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
		A Ø 2.7 mm	A Ø 3.5 mm	A Ø 3.9 mm	A Ø 4.6 mm	
Article		Art. No.				L
 <p><b>CONELOG® SCREW-LINE Implant, Promote® plus</b> with snap-in insertion post</p>	-	C1066.3807	C1066.4307	C1066.5007	7 mm	
	C1066.3309	C1066.3809	C1066.4309	C1066.5009	9 mm	
	C1066.3311	C1066.3811	C1066.4311	C1066.5011	11 mm	
	C1066.3313	C1066.3813	C1066.4313	C1066.5013	13 mm	
	C1066.3316	C1066.3816	C1066.4316	C1066.5016	16 mm	
 <p><b>CONELOG® SCREW-LINE Implant, Promote® plus</b> with screw-mounted insertion post</p>	-	C1065.3807	C1065.4307	C1065.5007	7 mm	
	C1065.3309	C1065.3809	C1065.4309	C1065.5009	9 mm	
	C1065.3311	C1065.3811	C1065.4311	C1065.5011	11 mm	
	C1065.3313	C1065.3813	C1065.4313	C1065.5013	13 mm	
	C1065.3316	C1065.3816	C1065.4316	C1065.5016	16 mm	






# Prosthetic overview


## Scanbodies

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	CONELOG® Scanbody	C2600.3310	C2600.4310	C2600.4310	C2600.5010	-
	CONELOG® ScanPost for Sirona® Scanbody	C2620.3306	C2620.3806	C2620.4306	C2620.5006	-




## Implant impression taking

	CONELOG® Impression post, open tray	C2121.3300	C2121.3800	C2121.4300	C2121.5000	-
	CONELOG® Impression post, closed tray	C2110.3300	C2110.3800	C2110.4300	C2110.5000	-
	Impression cap for impression posts, closed tray	J2111.3300	J2111.3800	J2111.4300	J2111.5000	-





## Bite registration

	CONELOG® Bite registration post incl. bite registration cap	C2140.3300	C2140.3800	C2140.4300	C2140.5000	-
---	---	------------	------------	------------	------------	---

## Cast fabrication









		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	<b>CONELOG® Lab analog</b> for cast models	C3010.3300	C2211.3300	C3010.4300	C3010.5000	-
		C3010.3303	C3010.3803	C3010.4303	C3010.5003	
	<b>CONELOG® Implant analog</b> for printed and cast models	C3025.3300	C3025.3800	C3025.4300	C3025.5000	-
		C3025.3303	C3025.3803	C3025.4303	C3025.5003	
	<b>DIM Analog® for the CONELOG® Implant System</b> for printed models	C3012.3300	C3012.4300	C3012.4300	C3012.5000	-

## Abutments for crown and bridge restorations
















	<b>CONELOG® Temporary abutment, crown, titanium alloy</b>	C2239.3300	C2239.3800	C2239.4300	C2239.5000	-
	<b>CONELOG® Temporary abutment, bridge, titanium alloy</b>	C2339.3300	C2339.3800	C2339.4300	C2339.5000	-
	<b>CONELOG® Titanium base CAD/CAM, crown</b>	C2242.3308	C2242.3808	C2242.4308	C2242.5008	0.8 mm
		C2242.3320	C2242.3820	C2242.4320	C2242.5020	2.0 mm
	<b>CONELOG® Titanium base CAD/CAM, bridge</b>	C2342.3308	C2342.3808	C2342.4308	C2342.5008	0.8 mm
		C2342.3320	C2342.3820	C2342.4320	C2342.5020	2.0 mm
	<b>CONELOG® CAM titanium blank, type IAC</b>	C2431.3313	C2431.3813	C2431.4313	C2431.5013	
	<b>CONELOG® CAM titanium blank, type ME</b>	C2441.3320	C2441.3820	C2441.4320	C2441.5020	
	<b>CONELOG® CAM CoCr blank, type ME</b>	C2461.3320	-	C2461.4320	C2461.5020	

# Prosthetic overview

## Abutments for crown and bridge restorations

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	CONELOG® Esthomic® Abutments, straight	-	C2226.3815	C2226.4315	C2226.5015	1.5–2.5 mm
		-	C2226.3830	C2226.4330	C2226.5030	3.0–4.5 mm
	CONELOG® Esthomic® Abutment, Inset	C2235.3320	C2235.3820	C2235.4320	C2235.5020	2.0–3.3 mm
	CONELOG® Esthomic® Abutments 15° angled, type A	-	C2227.3815	C2227.4315	C2227.5015	1.5–2.5 mm
		-	C2227.3830	C2227.4330	C2227.5030	3.0–4.5 mm
	CONELOG® Esthomic® Abutments 15° angled, type B	-	C2228.3815	C2228.4315	C2228.5015	1.5–2.5 mm
		-	C2228.3830	C2228.4330	C2228.5030	3.0–4.5 mm
	CONELOG® Esthomic® Abutments 20° angled, type A	-	C2231.3815	C2231.4315	C2231.5015	1.5–2.5 mm
		-	C2231.3830	C2231.4330	C2231.5030	3.0–4.5 mm
	CONELOG® Esthomic® Abutments 20° angled, type B	-	C2232.3815	C2232.4315	C2232.5015	1.5–2.5 mm
		-	C2232.3830	C2232.4330	C2232.5030	3.0–4.5 mm
	CONELOG® Universal abutment	C2211.3300	C2211.3800	C2211.4300	C2211.5000	-
	CONELOG® Gold-plastic abutment	C2246.3300	C2246.3800	C2246.4300	C2246.5000	-





## COMFOUR® Abutments for crown, bridge and hybrid restorations

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	CONELOG® Bar abutments, straight	C2254.3310	C2254.3810	C2254.4310	C2254.5010	1.0 mm
		C2254.3325	C2254.3825	C2254.4325	C2254.5025	2.5 mm
		-	C2254.3840	C2254.4340	C2254.5040	4.0 mm
	CONELOG® Bar abutments, 17° angled, type A	C2256.3325	C2256.3825	C2256.4325	C2256.5025	2.5 mm
		C2256.3340	C2256.3840	C2256.4340	C2256.5040	4.0 mm
	CONELOG® Bar abutments, 17° angled, type B	C2257.3325	C2257.3825	C2257.4325	C2257.5025	2.5 mm
		C2257.3340	C2257.3840	C2257.4340	C2257.5040	4.0 mm
	CONELOG® Bar abutments, 30° angled, type A	C2258.3325	C2258.3825	C2258.4325	C2258.5035	2.5 mm/ 3.5 mm*
		C2258.3340	C2258.3840	C2258.4340	C2258.5050	4.0 mm/ 5.0 mm*
	CONELOG® Bar abutments, 30° angled, type B	C2259.3325	C2259.3825	C2259.4325	C2259.5035	2.5 mm/ 3.5 mm*
		C2259.3340	C2259.3840	C2259.4340	C2259.5050	4.0 mm/ 5.0 mm*
	Healing cap for bar abutment	J2029.4300	J2029.4300	J2029.4300	J2029.6000	-
	Impression cap, short for bar abutment, closed tray	J2129.4300	J2129.4300	J2129.4300	J2129.6000	-
	Impression cap, long, for bar abutment, closed tray (bridge/bar)	J2129.4310	J2129.4310	J2129.4310	J2129.6010	-
	Scanning cap for bar abutments	J2610.4300	J2610.4300	J2610.4300	J2610.6000	-
	Titanium cap for bar abutment, for crown, sterile	J2259.4301	J2259.4301	J2259.4301	J2259.6001	-
	Titanium cap for bar abutment, for bridge, sterile	J2259.4302	J2259.4302	J2259.4302	J2259.6002	-
	Titanium cap without retention for bar abutment, for bridge	J2259.4322	J2259.4322	J2259.4322	J2259.6022	-
	Crown base for bar abutment, burn-out	J2256.4306	J2256.4306	J2256.4306	J2256.6006	-
	Base for bar abutment, burn-out	J2257.4301	J2257.4301	J2257.4301	J2257.6001	-
	Base for bar abutment, cast-on	J2263.4300	J2263.4300	J2263.4300	J2263.6000	-














\* GH 3.5 and 5.0 mm only for Ø 5.0 mm

# Prosthetic overview

## COMFOUR® Abutments for crown, bridge and hybrid restorations








		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
	Base for bar abutment, solderable	J2258.4300	J2258.4300	J2258.4300	J2258.6000	-
	Base for bar abutment, titanium, laser-weldable	J2262.4300	J2262.4300	J2262.4300	J2262.6000	-
	Titanium bonding base for bar abutment, Passive-Fit	J2260.4301	J2260.4301	J2260.4301	J2260.6001	-
	Bar sleeve for titanium bonding base, burn-out, Passive-Fit	J2261.4301	J2261.4301	J2261.4301	J2261.6001	-

## Hybrid restorations

	CONELOG® Ball abutment, male part	C2249.3315	C2249.3815	C2249.4315	C2249.5015	1.5 mm
		C2249.3330	C2249.3830	C2249.4330	C2249.5030	3.0 mm
		-	C2249.3845	C2249.4345	C2249.5045	4.5 mm
	CM Dalbo®-Plus matrix	05003503	05003503	05003503	05003503	-
	Ball abutment analog	C3015.3300	C3015.3300	C3015.3300	C3015.5000	-
	CONELOG® Locator R-Tx® Abutment	30805-01	30806-01	30807-01	30808-01	1.0 mm
		30805-02	30806-02	30807-02	30808-02	2.0 mm
		30805-03	30806-03	30807-03	30808-03	3.0 mm
		30805-04	30806-04	30807-04	30808-04	4.0 mm
		-	30806-05	30807-05	30808-05	5.0 mm
	Locator R-Tx® Impression cap	30017-01	30017-01	30017-01	30017-01	-
	Locator R-Tx® Analog	30014-01	30014-01	30014-01	30016-01	-
	Locator R-Tx® Retention housing	30013-01	30013-01	30013-01	30013-01	-
	Locator R-Tx® Processing replacement male	30012-01	30012-01	30012-01	30012-01	-
	Locator R-Tx® Spacer/duplication aid	30018-01	30018-01	30018-01	30018-01	-
	Locator R-Tx® Replacement male gray, NO RETENTION	30001-01	30001-01	30001-01	30001-01	-
	Locator R-Tx® Replacement male, blue, LOW	30002-01	30002-01	30002-01	30002-01	-
	Locator R-Tx® Replacement male, pink, MEDIUM	30003-01	30003-01	30003-01	30003-01	-
	Locator R-Tx® Replacement male, white, HIGH	30004-01	30004-01	30004-01	30004-01	-























## Hybrid restorations

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
Article		Art. No.				GH
 <b>CONELOG®</b> <b>Locator® Abutment</b>	C2253.3310	C2253.3810	C2253.4310	C2253.5010	1.0 mm	
	C2253.3320	C2253.3820	C2253.4320	C2253.5020	2.0 mm	
	C2253.3330	C2253.3830	C2253.4330	C2253.5030	3.0 mm	
	C2253.3340	C2253.3840	C2253.4340	C2253.5040	4.0 mm	
	-	C2253.3850	C2253.4350	C2253.5050	5.0 mm	
 <b>Locator® Impression cap</b>	J2253.0200	J2253.0200	J2253.0200	J2253.0200	-	
 <b>Locator® Analog</b>	J2253.0340	J2253.0340	J2253.0340	J2253.0340	-	
 <b>Locator® Lab kit</b>	J2253.0102	J2253.0102	J2253.0102	J2253.0102	-	
 <b>Locator® Lab kit, for extended angulation</b>	-	J2253.0112	J2253.0112	J2253.0112	-	
 <b>CONELOG®</b> <b>Universal abutment</b>	-	C2211.3800	C2211.4300	C2211.5000	-	
 <b>CONELOG®</b> <b>Telescope abutment</b>	-	C2212.3800	C2212.4300	C2212.5000	-	

# Screw overview Abutment and prosthetic screws – intraoral use

## Implant-abutment connection






	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
	M1.6			M2.0	
Article	CONELOG® Abutment screws				Tightening torque
 <p>Scanbodies ScanPost for Sirona® Scanbody</p>					hand-tight**
 <p>Temporary abutments titanium, crown and bridge</p>					
 <p>Esthomic® Abutments</p>					20 Ncm*
 <p>Universal abutment</p>	8.9 mm  C4005.1601		8.9 mm  C4005.2001		
 <p>Telescope abutment</p>					
 <p>Gold-plastic abutment</p>					
 <p>Logfit® Abutment</p>					
 <p>Vario SR abutments, 20° and 30° angled</p>					
 <p>CONELOG® CAM blank, type IAC and ME</p>					
<b>CONELOG® Abutment screws for titanium base CAD/CAM, anodized dark purple</b>					
 <p>Titanium base CAD/CAM, crown and bridge</p>	8.9 mm  C4015.1601		8.9 mm  C4015.2001		20 Ncm*
<b>CONELOG® Vario SR abutment screws</b>					
 <p>Vario SR abutment, straight</p>	10.6 mm  C4007.1600		10.6 mm  C4007.2000		20 Ncm*
<b>CONELOG® Abutment screws with reduced head, light blue anodized</b>					
 <p>COMFOUR® Bar abutments, 17° and 30° angled</p>	7.8 mm  C4004.1601		7.8 mm  C4004.2001		20 Ncm*

\* with torque wrench J5320.1030

\*\* optional for temporary abutments titanium: torque after completed healing phase 20 Ncm













**All screws must be retightened with the corresponding torque after at least 5 minutes!**

## Abutment-Prosthetic connection

		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm			
		M1.6			M2.0			
Article		Prosthetic screws for bar abutments, light blue anodized				Tightening torque		
 <p><b>COMFOUR®</b> Bar abutments, straight, 17° and 30° angled</p>	3.6 mm	 J4012.1601		3.8 mm	 J4012.2001		15 Ncm*	
	Vario SR prosthetic screw, yellow anodized							
 <p><b>Vario SR abutments,</b> straight, 20° and 30° angled</p>	4 mm		 J4005.2004				15 Ncm*	

## Overview Auxiliary Screws intra and extraoral use

### Abutment-Prosthetic connection





















		Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm			
		M1.6			M 2.0			
Article		Prosthetic screws for bar abutments, light blue anodized				Tightening torque		
 <p><b>Scanning cap for bar abutments</b></p>	3.6 mm	 J4012.1601		3.8 mm	 J4012.2001		hand-tight	
Screws for bar abutments, for open tray impression taking and for soldering, light blue anodized								
 <p><b>COMFOUR®</b> Bar abutments, straight, 17° and 30° angled</p>	12 mm	 J4012.1610		12.2 mm	 J4012.2010		hand-tight	
	17 mm	 J4012.1615		17.2 mm	 J4012.2015			
	22 mm	 J4012.1620		22.2 mm	 J4012.2020			
	Plastic screws for bar abutment, as fixation and bonding aid, beige							
	29 mm	 J4009.1627		29.2 mm	 J4009.2027		hand-tight	

\* with torque wrench J5320.1030

All screws must be retightened with the corresponding torque after at least 5 minutes!

# Screw Overview lab screws – extraoral use












## Lab analog-abutment connection

	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
	M1.6			M2.0	
Article	CONELOG® Lab screws*, brown anodized				Tightening torque
 <p>Scanbodies ScanPost for Sirona® Scanbody</p>					hand-tight
 <p>Temporary abutments titanium, crown and bridge</p>					
 <p>Esthomic® Abutments</p>	8.9 mm  C4006.1601			8.9 mm  C4006.2001	
 <p>Universal abutment Telescope abutment Gold-plastic abutment</p>					
 <p>Vario SR abutments, 20° and 30° angled</p>					
 <p>CONELOG® CAM blank, type IAC and ME</p>					
<b>CONELOG® Lab screws* for titanium base CAD/CAM brown, partially anodized</b>					
 <p>Titanium base CAD/CAM, crown and bridge</p>	8.9 mm  C4016.1601			8.9 mm  C4016.2001	hand-tight
<b>CONELOG® Bonding aids**</b>					
 <p>Titanium base CAD/CAM, crown and bridge</p>	26 mm 			26 mm 	hand-tight
<b>CONELOG® Vario SR lab screws*, brown anodized</b>					
 <p>Vario SR abutment, straight</p>	10.6 mm  C4008.1600			10.6 mm  C4008.2000	hand-tight
<b>CONELOG® Lab screws* with reduced head, light blue partially anodized</b>					
 <p>COMFOUR® Bar abutments, 17° and 30° angled</p>	7.8 mm  C4004.1600			7.8 mm  C4004.2000	hand-tight

\* Lab screws must not be used on patients!













\*\* not available singly, are included in the packaging of the titanium base CAD/CAM

## Abutment-Prosthetic connection

	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	
	M1.6			M2.0	
Article	Lab prosthetic screws* for bar abutments, brown anodized				Tightening torque
 Scanning cap for bar abutments					hand-tight
 <b>COMFOUR®</b> Bar abutments, straight, 17° and 30° angled	3.6 mm  J4013.1601	3.8 mm  J4013.2001			
 Bar lab analog for bar abutments					
<b>Vario SR prosthetic screw, yellow anodized</b>					
 Vario SR abutments, straight, 20° and 30° angled	4 mm  J4005.2004				hand-tight
 Vario SR analog					
<b>Prosthetic screws for bar abutments*, for fabricating the wax-up on the burn-out bar sleeve for titanium adhesive base, Passive-Fit, on the bar lab analog</b>					
 Titanium bonding base for bar abutment and bar sleeve for titanium bonding base, burn-out, Passive-Fit	5.5 mm  J4005.1602	5.5 mm  J4005.2002		hand-tight	

\* Lab screws must not be used on patients!






























# Overview tightening torques

Article	Instrument	Tightening torque
 <p>Implant cover screw</p>		
 <p>Healing caps cylindrical, wide body, bottleneck</p>		
 <p>Impression posts Bite registration posts</p>		hand-tight**
 <p>Lab screws Lab screws with reduced head</p>		
 <p>Temporary abutment, titanium alloy, crown and bridge</p>		
 <p>Abutment screws Abutment screws with reduced head</p>	 <p>J5317.0510    J5317.0501    J5317.0502</p>	
 <p>Esthomic® Abutment, straight Esthomic® Abutment, 15° and 20° angled Esthomic® Abutment, Inset</p>	 <p>J5317.0504    J5317.0503</p>	
 <p>Universal abutment Telescope abutment Gold-plastic abutment</p>		20 Ncm*
 <p>Logfit® Abutments Titanium bases CAD/CAM, crown and bridge</p>		
 <p>CONELOG® CAM blank, type IAC and ME</p>		

\* with the torque wrench J5320.1030

\*\* optional for temporary abutments titanium: torque after completed healing phase 20 Ncm

**All screws must be retightened with the corresponding torque after at least 5 minutes!**

	Ø 3.3 mm	Ø 3.8 mm	Ø 4.3 mm	Ø 5.0 mm	3.3	3.8	4.3	5.0
Article	Instrument				Tightening torque			
 Bar abutments, straight					20 Ncm*	30 Ncm*		
 Bar abutments, 17° and 30° angled					20 Ncm*			
 Scanning cap for bar abutment					hand-tight			
 Titanium caps for bar abutment, crown/bridge					15 Ncm*			
 Crown base for bar abutment, burn-out								
 Bar bases for bar abutment, burn-out, cast-on, solderable, laser-weldable								
 Titanium bonding base for bar abutment, Passive-Fit								
 Locator R-Tx® Abutments								
 Healing cap for bar abutment					hand-tight			
 Impression cap for bar abutment, closed tray (bridge/bar)								
 Ball abutments					20 Ncm*	30 Ncm*		
 Locator® Abutments					20 Ncm*			
 Locator® Fixture for bar abutment								
 Scanbodies					hand-tight			
 ScanPost for Sirona® Scanbody								

\* with torque wrench J5320.1030

All screws must be retightened with the corresponding torque after at least 5 minutes!

# Materials

Titanium Grade 4		
Properties (ASTM F67 and DIN EN ISO 5832-2)		
Chemical structure (in %)	O	≤ 0.4
	Fe	≤ 0.5
	C	≤ 0.08
	N	≤ 0.05
	H	≤ 0.0125
	Ti	Rest
Mechanical properties	Tensile strength	≥ 550 MPa
	Elongation at break	≥ 12 %

Titanium alloy Ti-6Al-4V ELI		
Properties (ASTM F136)		
Chemical structure (in %)	Al	5.5–6.5
	V	3.5–4.5
	Fe	≤ 0.25
	C	≤ 0.08
	N	≤ 0.05
	O	≤ 0.13
	H	≤ 0.012
	Ti	Rest
Mechanical properties	Tensile strength	≥ 860 MPa
	Elongation at break	≥ 10 %

Cast-on gold alloy CONELOG® Gold-plastic abutment		
Properties		
Chemical structure (in %)	Au	60
	Pd	20
	Pt	19
	Ir	1
Physical properties	Melting range	1400–1490 °C
	Density	17.5 g/cm <sup>3</sup>
	Modulus of elasticity	136 GPa
	Coefficient of thermal expansion (25–500 °C)	11.9 µm/m × °C
	Coefficient of thermal expansion (25–600 °C)	12.2 µm/m × °C
	Color	white
Mechanical properties	Status	cold-formed
	Hardness HV5	> 215
	Tensile strength (Rm)	> 750 MPa
	0.2 % Elongation limit (Rp 0.2 %)	> 650 MPa
	Elongation at break	> 2 %

Cast-on gold alloy bar base for bar abutment		
Properties		
Chemical structure (in %)	Au	60
	Pt	19
	Pd	20
	Ir	1
Physical properties	Density	17.5 g/cm <sup>3</sup>
	Color	white
	Liquidus	1490 °C
	Solidus	1400 °C
	Coefficient of thermal expansion (25–500 °C)	12.5 µm/m × °C
	Coefficient of thermal expansion (25–600 °C)	12.6 µm/m × °C
Mechanical properties	Modulus of elasticity	136 GPa
	Hardness HV5	210
	0.2 % Elongation limit	450–570 MPa
	Elongation at break	min. 10 %
	Tensile strength MPa	530–650



Solderable gold alloy bar base for bar abutment		
Properties		
Chemical structure (in %)	Au	68.60
	Pt	2.45
	Ag	11.85
	Pd	3.95
	Cu	10.60
	Zn	2.50
	Ir	0.05
	Rh	-
	Ru	-
	Physical properties	Color
Melting range		880–940 °C
Mechanical properties	Hardness annealed HV5	175
	hardened HV5	275
	self-hardened HV5	240

CoCr alloy		
Properties (ASTM F1537-20 and ISO 5832-12)		
Chemical structure (in wt %)	Cr	26.0–30.0
	Mo	5.0–7.0
	Fe	≤ 0.75
	Ni	≤ 0.1*
	Mn	< 1.0
	Si	< 1.0
	N	< 0.25
	C	≤ 0.14
	Co	Rest
	Physical properties	Coefficient of thermal expansion (25–500 °C)
Mechanical properties	Tensile strength	> 827 MPa
	Breaking strength	1172–1400 MPa
	Elongation at break	> 12 %
	Hardness (HRC)	38–48

\* ASTM F1537-20 and ISO 5832-12: ≤ 1.0 weight-%

# Index alphabetical

<b>A</b>		<b>C</b>	
Abutment collets	92	Collet for CAM blank, type IAC	71
Abutment screw for CONELOG® Titanium base CAD/CAM	69	COMFOUR® Patient brochure	98
Abutment screw with reduced head	78	Countersink	50
Abutment screw, hex	87	Crown base for bar abutment	77
Adapter, ISO shaft	53	<b>D</b>	
Aligning tool	76	Demonstration models, acrylic glass	97
Appointment pad	99	Dense bone drill PROGRESSIVE-LINE	25, 36
<b>B</b>		Depth stop for form drills PROGRESSIVE-LINE and SCREW-LINE	25, 43
Ball abutment analog	81	Depth stop SCREW-LINE for pilot drills and pre-drills	50
Ball abutment, male part	81	DIM Analog® for the CONELOG® Implant System	66
Bar abutments	75	Disconnecter	91
Bar implant analog for bar abutments	76	Drill extension, ISO shaft (not for drills with internal irrigation)	51
Bar lab analog for bar abutments	76	Drill extension, ISO shaft, for instruments with internal irrigation	47
Bar sleeve for titanium bonding base	77	Drills for placement of corrugated CT-tubes	19
Baring drill for cover screw	50	Drills PROGRESSIVE-LINE Flex	36
Base for bar abutment	77	<b>E</b>	
Base for bar abutment, titanium	77	Edentulous mandible	97
Biomaterial patient brochure	98	EP pilot drill set	44
Bite registration cap	66	Esthomic® Abutments	72, 73
Bite registration posts	66	Esthomic® Abutments, Inset	72
Bone profiler	50	<b>F</b>	
<b>C</b>		Form drills PROGRESSIVE-LINE	25
CAM blanks	70	Form drills SCREW-LINE	43
Cleaning cannula	55	Form drills SCREW-LINE cortical bone	43
Cleaning needle	55		
CM Dalbo®-Plus matrix	81		

<b>G</b>		<b>I</b>	
Gingiva height indicator, straight	76	Implants for practice	96
Gold-plastic abutment	74	<b>Implants</b>	
Guide System dense bone drill PROGRESSIVE-LINE	32	CONELOG® PROGRESSIVE-LINE Promote® plus	21
Guide System form drill for Ø 3.8 mm underpreparation PROGRESSIVE-LINE	32	CONELOG® SCREW-LINE Implant, Promote® plus	38, 39
Guide System form drill PROGRESSIVE-LINE	31	Impression cap for bar abutment, closed tray	76
Guide System form drill SCREW-LINE cortical bone	47	Impression cap for impression post, closed tray	65
Guide System gingiva punch PROGRESSIVE-LINE	31	Impression posts PS	67
Guide System gingiva punch	47	Impression posts	65
Guide System guiding sleeve PROGRESSIVE-LINE	32	Insertion aid	54
Guide System guiding sleeve	47	Insertion post, screw-mounted	96
Guide System pilot drill PROGRESSIVE-LINE	31	Insertion tool for ball abutment	88
Guide System pilot drill set	46	Insertion tool for impression posts and healing caps for bar abutments	76, 89
Guide System pre-drill PROGRESSIVE-LINE	31	Insertion tool for Locator®	89
Guide System pattern for surgery wash tray CAMLOG®/CONELOG® PROGRESSIVE-LINE	30	Insertion tool for screw implants	52
Guide System surgery set SCREW-LINE	46	Insertion tool for straight bar abutments	88, 89
Guide System surgery tray CAMLOG®/CONELOG® PROGRESSIVE-LINE	30		
Guide System surgery wash tray CAMLOG®/CONELOG® PROGRESSIVE-LINE	30	<b>L</b>	
Guiding pin for bone profiler	50	Lab analog	66
		Lab prosthetic screw for bar abutment	78
		Lab screw for CONELOG® Titanium base CAD/CAM	69
		Lab screw with reduced head	78
		Lab screw, hex	87
		Lamella retention insert	81
		Locator R-Tx® Abutment	82
		Locator R-Tx® Analog	82
		Locator R-Tx® Impression cap	82
		Locator R-Tx® Insertion tool for replacement males	90
		Locator R-Tx® Processing replacement male	83
<b>H</b>			
Handle for CAMLOG®/CONELOG® Implant analog	92		
Healing cap for bar abutment	76		
Healing caps	62		
<b>I</b>			
Implant analog	66		
Implant cover screw	62		

# Index alphabetical

<b>L</b>		<b>P</b>	
Locator R-Tx® Replacement male	83	Paralleling pin PROGRESSIVE-LINE	25
Locator R-Tx® Retention housing	83	Paralleling pin SCREW-LINE	51
Locator R-Tx® Spacer/duplication aid	83	Patient advice sheets	98
Locator® Abutment holder sleeve	89	Patient brochures	98
Locator® Abutment	84	Patient Documentation and Implant Card	98
Locator® Analog	84	Patient flyer	100
Locator® Angle measurement guide	89	<b>Patterns for surgery and wash tray</b>	
Locator® Block out spacer	85	CAMLOG®/CONELOG® PROGRESSIVE-LINE	24
Locator® Impression cap	84	CAMLOG®/CONELOG® PROGRESSIVE-LINE Guide System	30
Locator® Instrument	89	CAMLOG®/CONELOG® SCREW-LINE	42
Locator® Lab kits for extended angulation	85	PickUp instrument	53
Locator® Lab kits	85	Pilot drill SCREW-LINE	49
Locator® Parallel post	89	Pilot drills	49
Locator® Processing replacement male	85	Plastic screw for bar abutment	79
Locator® Replacement male for extended angulation	86	Point drill	49
Locator® Replacement male	86	Polishing protection for caps and bases for bar abutment	78
		Poster	99
		Pre-drill SCREW-LINE	49
		Pre-Osteotome SCREW-LINE	57, 58, 59, 60
		Presentation folder	99
		Profile drill PROGRESSIVE-LINE Flex	36
		Prosthetic screw for bar abutment	78
		Prosthetic tray Universal	90
		Prosthetic tray	90
		<b>R</b>	
		Removal adapter for CAMLOG® and CONELOG®	51
		Reworking reamer, base for bar abutment	92
		Round bur	49

<b>S</b>		<b>T</b>	
<hr/>		<hr/>	
Scanbodies	64	Titanium base CAD/CAM, crown	68
Scanning cap for bar abutments	76	Titanium bonding base for bar abutment	77
ScanPost for Sirona® Scanbody	64	Titanium cap for bar abutment, for bridge	77
Screw, hex	79	Titanium cap for bar abutment, for crown	77
Screwdriver activator	88	Titanium cap without retention for bar abutment, for bridge	77
Screwdriver, hex, ISO shaft	55, 91	Torque wrench	53, 88
Screwdriver, hex, manual/wrench	54, 90	Tubing for CT planning	19
SCREW-LINE EP form drill	44		
SCREW-LINE EP pre-drill	44	<b>U</b>	
Selection abutment kit	93	<hr/>	
Sleeve for inserting the insertion aid into the implant	54	Universal abutment	74, 87
<b>Surgery sets</b>		Universal holder	91
CAMLOG®/CONELOG® PROGRESSIVE-LINE	24	Universal holding key	54
CAMLOG®/CONELOG® PROGRESSIVE-LINE Flex	35		
CAMLOG®/CONELOG® SCREW-LINE	42	<b>W</b>	
<b>Surgery tray</b>		<hr/>	
CAMLOG®/CONELOG® PROGRESSIVE-LINE Guide System	30	Wrench adapter	36
<b>Surgery wash trays</b>			
CAMLOG®/CONELOG® PROGRESSIVE-LINE	24	<b>X</b>	
CAMLOG®/CONELOG® PROGRESSIVE-LINE Guide System	30	<hr/>	
CAMLOG®/CONELOG® SCREW-LINE	42	X-Ray Planning foils	18
		X-Ray Transfer pictures 1.25:1, CONELOG® SCREW-LINE implants	18
<b>T</b>			
<hr/>			
Tap adapter	51		
Tap PROGRESSIVE-LINE	25, 36		
Tap SCREW-LINE	43		
Telescope abutment for the double crown technique	87		
Temporary abutment, bridge, titanium alloy	67		
Temporary abutment, crown, titanium alloy	67		
Titanium base CAD/CAM, bridge	68		

# Index Article Number

05003503	CM Dalbo®-Plus matrix	81			
05003504	Lamella retention insert	81			
07000389	Screwdriver activator	88			
08394	Locator® Abutment holder sleeve	89			
	<b>Locator R-Tx® Replacement male</b>				
30001-01	Ø 3.3/3.8/4.3/5.0 mm, gray, NO RET.	83	C1065.3309	Ø 3.3 mm, L 9 mm	39
30002-01	Ø 3.3/3.8/4.3/5.0 mm, blue, LOW	83	C1065.3311	Ø 3.3 mm, L 11 mm	39
30003-01	Ø 3.3/3.8/4.3/5.0 mm, pink, MEDIUM	83	C1065.3313	Ø 3.3 mm, L 13 mm	39
30004-01	Ø 3.3/3.8/4.3/5.0 mm, white, HIGH	83	C1065.3316	Ø 3.3 mm, L 16 mm	39
			C1065.3807	Ø 3.8 mm, L 7 mm	39
			C1065.3809	Ø 3.8 mm, L 9 mm	39
			C1065.3811	Ø 3.8 mm, L 11 mm	39
			C1065.3813	Ø 3.8 mm, L 13 mm	39
			C1065.3816	Ø 3.8 mm, L 16 mm	39
			C1065.4307	Ø 4.3 mm, L 7 mm	39
			C1065.4309	Ø 4.3 mm, L 9 mm	39
			C1065.4311	Ø 4.3 mm, L 11 mm	39
30012-01	Locator R-Tx® Processing replacement male	83	C1065.4313	Ø 4.3 mm, L 13 mm	39
			C1065.4316	Ø 4.3 mm, L 16 mm	39
			C1065.5007	Ø 5.0 mm, L 7 mm	39
30013-01	Locator R-Tx® Retention housing	83	C1065.5009	Ø 5.0 mm, L 9 mm	39
			C1065.5011	Ø 5.0 mm, L 11 mm	39
			C1065.5013	Ø 5.0 mm, L 13 mm	39
30014-01	Ø 3.3/3.8/4.3 mm	82			
30016-01	Ø 5.0 mm	82			
30017-01	Locator R-Tx® Impression cap	82	C1066.3309	Ø 3.3 mm, L 9 mm	38
			C1066.3311	Ø 3.3 mm, L 11 mm	38
30018-01	Locator R-Tx® Spacer/duplication aid	83	C1066.3313	Ø 3.3 mm, L 13 mm	38
			C1066.3316	Ø 3.3 mm, L 16 mm	38
30021-01	Locator R-Tx® Insertion tool for replacement males	90	C1066.3807	Ø 3.8 mm, L 7 mm	38
			C1066.3809	Ø 3.8 mm, L 9 mm	38
			C1066.3811	Ø 3.8 mm, L 11 mm	38
			C1066.3813	Ø 3.8 mm, L 13 mm	38
			C1066.3816	Ø 3.8 mm, L 16 mm	38
30805-01	Ø 3.3 mm, GH 1.0 mm	82	C1066.4307	Ø 4.3 mm, L 7 mm	38
30805-02	Ø 3.3 mm, GH 2.0 mm	82	C1066.4309	Ø 4.3 mm, L 9 mm	38
30805-03	Ø 3.3 mm, GH 3.0 mm	82	C1066.4311	Ø 4.3 mm, L 11 mm	38
30805-04	Ø 3.3 mm, GH 4.0 mm	82	C1066.4313	Ø 4.3 mm, L 13 mm	38
30806-01	Ø 3.8 mm, GH 1.0 mm	82	C1066.4316	Ø 4.3 mm, L 16 mm	38
30806-02	Ø 3.8 mm, GH 2.0 mm	82	C1066.5007	Ø 5.0 mm, L 7 mm	38
30806-03	Ø 3.8 mm, GH 3.0 mm	82	C1066.5009	Ø 5.0 mm, L 9 mm	38
30806-04	Ø 3.8 mm, GH 4.0 mm	82	C1066.5011	Ø 5.0 mm, L 11 mm	38
30806-05	Ø 3.8 mm, GH 5.0 mm	82	C1066.5013	Ø 5.0 mm, L 13 mm	38
30807-01	Ø 4.3 mm, GH 1.0 mm	82	C1066.5016	Ø 5.0 mm, L 16 mm	38
30807-02	Ø 4.3 mm, GH 2.0 mm	82			
30807-03	Ø 4.3 mm, GH 3.0 mm	82			
30807-04	Ø 4.3 mm, GH 4.0 mm	82			
30807-05	Ø 4.3 mm, GH 5.0 mm	82			
30808-01	Ø 5.0 mm, GH 1.0 mm	82	C1069.3813	Ø 3.8 mm, L 13 mm	96
30808-02	Ø 5.0 mm, GH 2.0 mm	82	C1069.4313	Ø 4.3 mm, L 13 mm	96
30808-03	Ø 5.0 mm, GH 3.0 mm	82			
30808-04	Ø 5.0 mm, GH 4.0 mm	82			
30808-05	Ø 5.0 mm, GH 5.0 mm	82			
A2002.2000	Tubing for CT planning	19			
	<b>Drill for placement of corrugated CT-tubes</b>				
A2050.2600	Ø 2.6 mm	19			
A2050.2800	Ø 2.8 mm	19			
A2222.2200	Tubing for CT planning	19			

	<b>PROGRESSIVE-LINE Implant, Promote® plus incl. screw-mounted insertion post</b>			
C1085.3309	Ø 3.3 mm, L 9 mm	21		
C1085.3311	Ø 3.3 mm, L 11 mm	21		
C1085.3313	Ø 3.3 mm, L 13 mm	21		
C1085.3316	Ø 3.3 mm, L 16 mm	21		
C1085.3807	Ø 3.8 mm, L 7 mm	21		
C1085.3809	Ø 3.8 mm, L 9 mm	21		
C1085.3811	Ø 3.8 mm, L 11 mm	21		
C1085.3813	Ø 3.8 mm, L 13 mm	21		
C1085.3816	Ø 3.8 mm, L 16 mm	21		
C1085.4307	Ø 4.3 mm, L 7 mm	21		
C1085.4309	Ø 4.3 mm, L 9 mm	21		
C1085.4311	Ø 4.3 mm, L 11 mm	21		
C1085.4313	Ø 4.3 mm, L 13 mm	21		
C1085.4316	Ø 4.3 mm, L 16 mm	21		
C1085.5007	Ø 5.0 mm, L 7 mm	21		
C1085.5009	Ø 5.0 mm, L 9 mm	21		
C1085.5011	Ø 5.0 mm, L 11 mm	21		
C1085.5013	Ø 5.0 mm, L 13 mm	21		
C1085.5016	Ø 5.0 mm, L 16 mm	21		
	<b>PROGRESSIVE-LINE Implant, Promote® plus incl. snap-in insertion post</b>			
C1086.3309	Ø 3.3 mm, L 9 mm	21		
C1086.3311	Ø 3.3 mm, L 11 mm	21		
C1086.3313	Ø 3.3 mm, L 13 mm	21		
C1086.3316	Ø 3.3 mm, L 16 mm	21		
C1086.3807	Ø 3.8 mm, L 7 mm	21		
C1086.3809	Ø 3.8 mm, L 9 mm	21		
C1086.3811	Ø 3.8 mm, L 11 mm	21		
C1086.3813	Ø 3.8 mm, L 13 mm	21		
C1086.3816	Ø 3.8 mm, L 16 mm	21		
C1086.4307	Ø 4.3 mm, L 7 mm	21		
C1086.4309	Ø 4.3 mm, L 9 mm	21		
C1086.4311	Ø 4.3 mm, L 11 mm	21		
C1086.4313	Ø 4.3 mm, L 13 mm	21		
C1086.4316	Ø 4.3 mm, L 16 mm	21		
C1086.5007	Ø 5.0 mm, L 7 mm	21		
C1086.5009	Ø 5.0 mm, L 9 mm	21		
C1086.5011	Ø 5.0 mm, L 11 mm	21		
C1086.5013	Ø 5.0 mm, L 13 mm	21		
C1086.5016	Ø 5.0 mm, L 16 mm	21		
	<b>PROGRESSIVE-LINE Implant for practice</b>			
C1901.3813	Ø 3.8 mm, L 13 mm	96		
C1901.4313	Ø 4.3 mm, L 13 mm	96		
	<b>Healing cap, bottleneck</b>			
C2011.3340	Ø 3.3 mm, GH 4.0 mm	62		
C2011.3840	Ø 3.8 mm, GH 4.0 mm	62		
C2011.3860	Ø 3.8 mm, GH 6.0 mm	62		
C2011.4340	Ø 4.3 mm, GH 4.0 mm	62		
C2011.4360	Ø 4.3 mm, GH 6.0 mm	62		
C2011.5040	Ø 5.0 mm, GH 4.0 mm	62		
C2011.5060	Ø 5.0 mm, GH 6.0 mm	62		
	<b>Healing cap, wide body</b>			
C2014.3340	Ø 3.3 mm, GH 4.0 mm	62		
C2014.3840	Ø 3.8 mm, GH 4.0 mm	62		
C2014.3860	Ø 3.8 mm, GH 6.0 mm	62		
C2014.4340	Ø 4.3 mm, GH 4.0 mm	62		
C2014.4360	Ø 4.3 mm, GH 6.0 mm	62		
C2014.5040	Ø 5.0 mm, GH 4.0 mm	62		
C2014.5060	Ø 5.0 mm, GH 6.0 mm	62		
	<b>Healing cap, cylindrical</b>			
C2015.3320	Ø 3.3 mm, GH 2.0 mm	62		
C2015.3340	Ø 3.3 mm, GH 4.0 mm	62		
C2015.3820	Ø 3.8 mm, GH 2.0 mm	62		
C2015.3840	Ø 3.8 mm, GH 4.0 mm	62		
C2015.3860	Ø 3.8 mm, GH 6.0 mm	62		
C2015.4320	Ø 4.3 mm, GH 2.0 mm	62		
C2015.4340	Ø 4.3 mm, GH 4.0 mm	62		
C2015.4360	Ø 4.3 mm, GH 6.0 mm	62		
C2015.5020	Ø 5.0 mm, GH 2.0 mm	62		
C2015.5040	Ø 5.0 mm, GH 4.0 mm	62		
C2015.5060	Ø 5.0 mm, GH 6.0 mm	62		
	<b>Implant cover screw</b>			
C2019.3300	Ø 3.3 mm	62		
C2019.3800	Ø 3.8 mm	62		
C2019.4300	Ø 4.3 mm	62		
C2019.5000	Ø 5.0 mm	62		
	<b>Insertion post, screw-mounted</b>			
C2026.3303	Ø 3.3 mm	96		
C2026.3803	Ø 3.8 mm	96		
C2026.4303	Ø 4.3 mm	96		
C2026.5003	Ø 5.0 mm	96		
	<b>Impression posts, closed tray</b>			
C2110.3300	Ø 3.3 mm	65		
C2110.3800	Ø 3.8 mm	65		
C2110.4300	Ø 4.3 mm	65		
C2110.5000	Ø 5.0 mm	65		
	<b>Impression posts, open tray</b>			
C2121.3300	Ø 3.3 mm	65		
C2121.3800	Ø 3.8 mm	65		
C2121.4300	Ø 4.3 mm	65		
C2121.5000	Ø 5.0 mm	65		
	<b>Bite registration posts</b>			
C2140.3300	Ø 3.3 mm	66		
C2140.3800	Ø 3.8 mm	66		
C2140.4300	Ø 4.3 mm	66		
C2140.5000	Ø 5.0 mm	66		
	<b>Universal abutment</b>			
C2211.3300	Ø 3.3 mm	74		
C2211.3800	Ø 3.8 mm	74, 87		
C2211.4300	Ø 4.3 mm	74, 87		
C2211.5000	Ø 5.0 mm	74, 87		

# Index Article Number

	<b>Telescope abutment for the double crown technique</b>				<b>Modeling aid for CONELOG® Titanium base CAD/CAM, crown</b>	
C2212.3800	Ø 3.8 mm	87		C2242.3302	Ø 3.3 mm	69
C2212.4300	Ø 4.3 mm	87		C2242.3802	Ø 3.8 mm	69
C2212.5000	Ø 5.0 mm	87		C2242.4302	Ø 4.3 mm	69
				C2242.5002	Ø 5.0 mm	69
	<b>Esthomic® Abutments, straight</b>				<b>Titanium base CAD/CAM, crown</b>	
C2226.3815	Ø 3.8 mm, GH 1.5–2.5 mm	72		C2242.3308	Ø 3.3 mm, GH 0.8 mm	68
C2226.3830	Ø 3.8 mm, GH 3.0–4.5 mm	72		C2242.3320	Ø 3.3 mm, GH 2.0 mm	68
C2226.4315	Ø 4.3 mm, GH 1.5–2.5 mm	72		C2242.3808	Ø 3.8 mm, GH 0.8 mm	68
C2226.4330	Ø 4.3 mm, GH 3.0–4.5 mm	72		C2242.3820	Ø 3.8 mm, GH 2.0 mm	68
C2226.5015	Ø 5.0 mm, GH 1.5–2.5 mm	72		C2242.4308	Ø 4.3 mm, GH 0.8 mm	68
C2226.5030	Ø 5.0 mm, GH 3.0–4.5 mm	72		C2242.4320	Ø 4.3 mm, GH 2.0 mm	68
	<b>Esthomic® Abutments, 15° angled</b>			C2242.5008	Ø 5.0 mm, GH 0.8 mm	68
C2227.3815	Ø 3.8 mm, GH 1.5–2.5 mm, type A	73		C2242.5020	Ø 5.0 mm, GH 2.0 mm	68
C2227.3830	Ø 3.8 mm, GH 3.0–4.5 mm, type A	73				
C2227.4315	Ø 4.3 mm, GH 1.5–2.5 mm, type A	73			<b>Gold-plastic abutment</b>	
C2227.4330	Ø 4.3 mm, GH 3.0–4.5 mm, type A	73		C2246.3300	Ø 3.3 mm	74
C2227.5015	Ø 5.0 mm, GH 1.5–2.5 mm, type A	73		C2246.3800	Ø 3.8 mm	74
C2227.5030	Ø 5.0 mm, GH 3.0–4.5 mm, type A	73		C2246.4300	Ø 4.3 mm	74
C2228.3815	Ø 3.8 mm, GH 1.5–2.5 mm, type B	73		C2246.5000	Ø 5.0 mm	74
C2228.3830	Ø 3.8 mm, GH 3.0–4.5 mm, type B	73				
C2228.4315	Ø 4.3 mm, GH 1.5–2.5 mm, type B	73			<b>Ball abutment, male part</b>	
C2228.4330	Ø 4.3 mm, GH 3.0–4.5 mm, type B	73		C2249.3315	Ø 3.3 mm, GH 1.5 mm	81
C2228.5015	Ø 5.0 mm, GH 1.5–2.5 mm, type B	73		C2249.3330	Ø 3.3 mm, GH 3.0 mm	81
C2228.5030	Ø 5.0 mm, GH 3.0–4.5 mm, type B	73		C2249.3815	Ø 3.8 mm, GH 1.5 mm	81
	<b>Esthomic® Abutments, 20° angled</b>			C2249.3830	Ø 3.8 mm, GH 3.0 mm	81
C2231.3815	Ø 3.8 mm, GH 1.5–2.5 mm, type A	73		C2249.3845	Ø 3.8 mm, GH 4.5 mm	81
C2231.3830	Ø 3.8 mm, GH 3.0–4.5 mm, type A	73		C2249.4315	Ø 4.3 mm, GH 1.5 mm	81
C2231.4315	Ø 4.3 mm, GH 1.5–2.5 mm, type A	73		C2249.4330	Ø 4.3 mm, GH 3.0 mm	81
C2231.4330	Ø 4.3 mm, GH 3.0–4.5 mm, type A	73		C2249.4345	Ø 4.3 mm, GH 4.5 mm	81
C2231.5015	Ø 5.0 mm, GH 1.5–2.5 mm, type A	73		C2249.5015	Ø 5.0 mm, GH 1.5 mm	81
C2231.5030	Ø 5.0 mm, GH 3.0–4.5 mm, type A	73		C2249.5030	Ø 5.0 mm, GH 3.0 mm	81
C2232.3815	Ø 3.8 mm, GH 1.5–2.5 mm, type B	73		C2249.5045	Ø 5.0 mm, GH 4.5 mm	81
C2232.3830	Ø 3.8 mm, GH 3.0–4.5 mm, type B	73				
C2232.4315	Ø 4.3 mm, GH 1.5–2.5 mm, type B	73			<b>Locator® Abutment</b>	
C2232.4330	Ø 4.3 mm, GH 3.0–4.5 mm, type B	73		C2253.3310	Ø 3.3 mm, GH 1.0 mm	84
C2232.5015	Ø 5.0 mm, GH 1.5–2.5 mm, type B	73		C2253.3320	Ø 3.3 mm, GH 2.0 mm	84
C2232.5030	Ø 5.0 mm, GH 3.0–4.5 mm, type B	73		C2253.3330	Ø 3.3 mm, GH 3.0 mm	84
	<b>Esthomic® Abutments, Inset</b>			C2253.3340	Ø 3.3 mm, GH 4.0 mm	84
C2235.3320	Ø 3.3 mm, GH 2.0–3.3 mm	72		C2253.3810	Ø 3.8 mm, GH 1.0 mm	84
C2235.3820	Ø 3.8 mm, GH 2.0–3.3 mm	72		C2253.3820	Ø 3.8 mm, GH 2.0 mm	84
C2235.4320	Ø 4.3 mm, GH 2.0–3.3 mm	72		C2253.3830	Ø 3.8 mm, GH 3.0 mm	84
C2235.5020	Ø 5.0 mm, GH 2.0–3.3 mm	72		C2253.3840	Ø 3.8 mm, GH 4.0 mm	84
	<b>Temporary abutment, crown, titanium alloy</b>			C2253.3850	Ø 3.8 mm, GH 5.0 mm	84
C2239.3300	Ø 3.3 mm	67		C2253.4310	Ø 4.3 mm, GH 1.0 mm	84
C2239.3800	Ø 3.8 mm	67		C2253.4320	Ø 4.3 mm, GH 2.0 mm	84
C2239.4300	Ø 4.3 mm	67		C2253.4330	Ø 4.3 mm, GH 3.0 mm	84
C2239.5000	Ø 5.0 mm	67		C2253.4340	Ø 4.3 mm, GH 4.0 mm	84
				C2253.4350	Ø 4.3 mm, GH 5.0 mm	84
				C2253.5010	Ø 5.0 mm, GH 1.0 mm	84
				C2253.5020	Ø 5.0 mm, GH 2.0 mm	84
				C2253.5030	Ø 5.0 mm, GH 3.0 mm	84
				C2253.5040	Ø 5.0 mm, GH 4.0 mm	84
				C2253.5050	Ø 5.0 mm, GH 5.0 mm	84



	<b>Bar abutments, straight</b>				<b>Titanium base CAD/CAM, bridge</b>	
C2254.3310	Ø 3.3 mm, GH 1.0 mm	75		C2342.3308	Ø 3.3 mm, GH 0.8 mm	68
C2254.3325	Ø 3.3 mm, GH 2.5 mm	75		C2342.3320	Ø 3.3 mm, GH 2.0 mm	68
C2254.3810	Ø 3.8 mm, GH 1.0 mm	75		C2342.3808	Ø 3.8 mm, GH 0.8 mm	68
C2254.3825	Ø 3.8 mm, GH 2.5 mm	75		C2342.3820	Ø 3.8 mm, GH 2.0 mm	68
C2254.3840	Ø 3.8 mm, GH 4.0 mm	75		C2342.4308	Ø 4.3 mm, GH 0.8 mm	68
C2254.4310	Ø 4.3 mm, GH 1.0 mm	75		C2342.4320	Ø 4.3 mm, GH 2.0 mm	68
C2254.4325	Ø 4.3 mm, GH 2.5 mm	75		C2342.5008	Ø 5.0 mm, GH 0.8 mm	68
C2254.4340	Ø 4.3 mm, GH 4.0 mm	75		C2342.5020	Ø 5.0 mm, GH 2.0 mm	68
C2254.5010	Ø 5.0 mm, GH 1.0 mm	75			<b>CAM titanium blank, type IAC</b>	
C2254.5025	Ø 5.0 mm, GH 2.5 mm	75		C2431.3313	Ø 3.3 mm	70
C2254.5040	Ø 5.0 mm, GH 4.0 mm	75		C2431.3813	Ø 3.8 mm	70
	<b>Bar abutments, 17° angled</b>			C2431.4313	Ø 4.3 mm	70
C2256.3325	Ø 3.3 mm, GH 2.5, type A	75		C2431.5013	Ø 5.0 mm	70
C2256.3340	Ø 3.3 mm, GH 4.0, type A	75			<b>CAM titanium blank, type ME</b>	
C2256.3825	Ø 3.8 mm, GH 2.5, type A	75		C2441.3320	Ø 3.3 mm	70
C2256.3840	Ø 3.8 mm, GH 4.0, type A	75		C2441.3820	Ø 3.8 mm	70
C2256.4325	Ø 4.3 mm, GH 2.5, type A	75		C2441.4320	Ø 4.3 mm	70
C2256.4340	Ø 4.3 mm, GH 4.0, type A	75		C2441.5020	Ø 5.0 mm	70
C2256.5025	Ø 5.0 mm, GH 2.5, type A	75			<b>CAM CoCr blank, type ME</b>	
C2256.5040	Ø 5.0 mm, GH 4.0, type A	75		C2461.3320	Ø 3.3 mm	70
C2257.3325	Ø 3.3 mm, GH 2.5, type B	75		C2461.4320	Ø 3.8/4.3 mm	70
C2257.3340	Ø 3.3 mm, GH 4.0, type B	75		C2461.5020	Ø 5.0 mm	70
C2257.3825	Ø 3.8 mm, GH 2.5, type B	75			<b>Scanbodies</b>	
C2257.3840	Ø 3.8 mm, GH 4.0, type B	75		C2600.3310	Ø 3.3 mm	64
C2257.4325	Ø 4.3 mm, GH 2.5, type B	75		C2600.4310	Ø 3.8/4.3 mm	64
C2257.4340	Ø 4.3 mm, GH 4.0, type B	75		C2600.5010	Ø 5.0 mm	64
C2257.5025	Ø 5.0 mm, GH 2.5, type B	75			<b>ScanPost for Sirona® Scanbody</b>	
C2257.5040	Ø 5.0 mm, GH 4.0, type B	75		C2620.3306	Ø 3.3 mm	64
	<b>Bar abutments, 30° angled</b>			C2620.3806	Ø 3.8 mm	64
C2258.3325	Ø 3.3 mm, GH 2.5, type A	75		C2620.4306	Ø 4.3 mm	64
C2258.3340	Ø 3.3 mm, GH 4.0, type A	75		C2620.5006	Ø 5.0 mm	64
C2258.3825	Ø 3.8 mm, GH 2.5, type A	75			<b>Lab analog</b>	
C2258.3840	Ø 3.8 mm, GH 4.0, type A	75		C3010.3300	Ø 3.3 mm	66
C2258.4325	Ø 4.3 mm, GH 2.5, type A	75		C3010.3303	Ø 3.3 mm (3 units)	66
C2258.4340	Ø 4.3 mm, GH 4.0, type A	75		C3010.3800	Ø 3.8 mm	66
C2258.5035	Ø 5.0 mm, GH 3.5, type A	75		C3010.3803	Ø 3.8 mm (3 units)	66
C2258.5050	Ø 5.0 mm, GH 5.0, type A	75		C3010.4300	Ø 4.3 mm	66
C2259.3325	Ø 3.3 mm, GH 2.5, type B	75		C3010.4303	Ø 4.3 mm (3 units)	66
C2259.3340	Ø 3.3 mm, GH 4.0, type B	75		C3010.5000	Ø 5.0 mm	66
C2259.3825	Ø 3.8 mm, GH 2.5, type B	75		C3010.5003	Ø 5.0 mm (3 units)	66
C2259.3840	Ø 3.8 mm, GH 4.0, type B	75			<b>DIM Analog® for the CONELOG® Implant System</b>	
C2259.4325	Ø 4.3 mm, GH 2.5, type B	75		C3012.3300	Ø 3.3 mm	66
C2259.4340	Ø 4.3 mm, GH 4.0, type B	75		C3012.3800	Ø 3.8 mm	66
C2259.5035	Ø 5.0 mm, GH 3.5, type B	75		C3012.4300	Ø 4.3 mm	66
C2259.5050	Ø 5.0 mm, GH 5.0, type B	75		C3012.5000	Ø 5.0 mm	66
	<b>Temporary abutment, bridge, titanium alloy</b>					
C2339.3300	Ø 3.3 mm	67				
C2339.3800	Ø 3.8 mm	67				
C2339.4300	Ø 4.3 mm	67				
C2339.5000	Ø 5.0 mm	67				

# Index Article Number

	<b>Ball abutment analog</b>				<b>Guiding pin for bone profiler</b>	
C3015.3300	Ø 3.3/3.8/4.3 mm	81		C5002.3300	Ø 3.3 mm	50
C3015.5000	Ø 5.0 mm	81		C5002.3800	Ø 3.8 mm	50
	<b>Implant analog</b>			C5002.4300	Ø 4.3 mm	50
C3025.3300	Ø 3.3 mm	66		C5002.5000	Ø 5.0 mm	50
C3025.3303	Ø 3.3 mm (3 units)	66			<b>Disconnecter, for CONELOG® Abutments</b>	
C3025.3800	Ø 3.8 mm	66		C5300.1601	Ø 3.3/3.8/4.3 mm, M1.6, short	91
C3025.3803	Ø 3.8 mm (3 units)	66		C5300.1603	Ø 3.3/3.8/4.3 mm, M1.6, long	91
C3025.4300	Ø 4.3 mm	66		C5300.2001	Ø 5.0 mm, M2.0, short	91
C3025.4303	Ø 4.3 mm (3 units)	66		C5300.2003	Ø 5.0 mm, M2.0, long	91
C3025.5000	Ø 5.0 mm	66			<b>X-Ray Planning foil</b>	
C3025.5003	Ø 5.0 mm (3 units)	66			<b>CONELOG® SCREW-LINE Implants</b>	
	<b>Universal holder, incl. lab screws and abutment collet</b>	92		C5300.9010	X-Ray Planning foil 1.25:1	18
				C5300.9011	X-Ray Planning foil 1.4:1	18
	<b>Abutment collets</b>				<b>X-Ray Planning foil</b>	
C3709.3300	Ø 3.3 mm	92			<b>CONELOG® PROGRESSIVE-LINE Implants</b>	
C3709.3800	Ø 3.8 mm	92		C5300.9014	X-Ray Planning foil 1.25:1	18
C3709.4300	Ø 4.3 mm	92		C5300.9015	X-Ray Planning foil 1.4:1	18
C3709.5000	Ø 5.0 mm	92			<b>X-Ray Transfer pictures 1.25:1</b>	
	<b>Collet for CAM blank, type IAC</b>				<b>CONELOG® SCREW-LINE Implants</b>	
C3720.3300	Ø 3.3 mm	71		C5300.9080	Ø 3.3 mm	18
C3720.4300	Ø 3.8/4.3 mm	71		C5300.9081	Ø 3.8 mm	18
C3720.5000	Ø 5.0 mm	71		C5300.9082	Ø 4.3 mm	18
	<b>Lab screw, with reduced head</b>			C5300.9083	Ø 5.0 mm	18
C4004.1600	Ø 3.3/3.8/4.3 mm, M1.6	78			<b>Insertion aid</b>	
C4004.2000	Ø 5.0 mm, M2.0	78		C5302.3310	Ø 3.3 mm, long	54
	<b>Abutment screw, with reduced head</b>			C5302.3311	Ø 3.3 mm, short	54
C4004.1601	Ø 3.3/3.8/4.3 mm, M1.6	78		C5302.4310	Ø 3.8/4.3 mm, long	54
C4004.2001	Ø 5.0 mm, M2.0	78		C5302.4311	Ø 3.8/4.3 mm, short	54
	<b>Abutment screw, hex</b>			C5302.5011	Ø 5.0 mm, short	54
C4005.1601	Ø 3.3/3.8/4.3 mm, M1.6	87			<b>Macro model</b>	
C4005.2001	Ø 5.0 mm, M2.0	87		C8010.1010	SCREW-LINE	97
	<b>Lab screw, hex</b>			C8010.1400	PROGRESSIVE-LINE	97
C4006.1601	Ø 3.3/3.8/4.3 mm, M1.6	87		C8011.1000	<b>Selection abutment kit</b>	93
C4006.1603	Ø 3.3/3.8/4.3 mm, M1.6 (3 units)	87			<b>Demonstration model, acrylic glass</b>	
C4006.2001	Ø 5.0 mm, M2.0	87		C8050.1040	Lower jaw	97
C4006.2003	Ø 5.0 mm, M2.0 (3 units)	87		C8070.1020	Upper jaw	97
	<b>Abutment screw for CONELOG® Titanium base CAD/CAM</b>				<b>Healing cap for bar abutment</b>	
C4015.1601	Ø 3.3/3.8/4.3 mm, M1.6	69		J2029.4300	Ø 3.3/3.8/4.3 mm	76
C4015.2001	Ø 5.0 mm, M2.0	69		J2029.6000	Ø 5.0 mm	76
	<b>Lab screw for CONELOG® Titanium base CAD/CAM</b>				<b>Impression cap for impression post, closed tray</b>	
C4016.1601	Ø 3.3/3.8/4.3 mm, M1.6	69		J2111.3300	Ø 3.3 mm	65
C4016.2001	Ø 5.0 mm, M2.0	69		J2111.3800	Ø 3.8 mm	65
				J2111.4300	Ø 4.3 mm	65
				J2111.5000	Ø 5.0 mm	65

	<b>Bite registration cap</b>				<b>Titanium cap for bar abutment</b>	
J2112.3300	Ø 3.3 mm	66		J2259.4301	Ø 3.3/3.8/4.3 mm, for crown	77
J2112.3800	Ø 3.8 mm	66		J2259.4302	Ø 3.3/3.8/4.3 mm, for bridge	77
J2112.4300	Ø 4.3 mm	66		J2259.6001	Ø 5.0 mm, for crown	77
J2112.5000	Ø 5.0 mm	66		J2259.6002	Ø 5.0 mm, for bridge	77
	<b>Impression cap for bar abutment, closed tray (bridge/bar)</b>				<b>Titanium cap without retention for bar abutment, for bridge</b>	
J2129.4300	Ø 3.3/3.8/4.3 mm, short	76		J2259.4322	Ø 3.3/3.8/4.3 mm	77
J2129.4310	Ø 3.3/3.8/4.3 mm, long	76		J2259.6022	Ø 5.0 mm	77
J2129.6000	Ø 5.0 mm, short	76			<b>Titanium bonding base for bar abutment</b>	
J2129.6010	Ø 5.0 mm, long	76		J2260.4301	Ø 3.3/3.8/4.3 mm	77
J2253.0001	<b>Insertion tool for Locator®</b>	89		J2260.6001	Ø 5.0 mm	77
J2253.0002	<b>Locator® Instrument</b>	89			<b>Bar sleeve for titanium bonding base</b>	
J2253.0003	<b>Locator® Angle measurement guide</b>	89		J2261.4301	Ø 3.3/3.8/4.3 mm	77
J2253.0004	<b>Locator® Parallel post</b>	89		J2261.6001	Ø 5.0 mm	77
J2253.0102	<b>Locator® Lab kits</b>	85			<b>Base for bar abutment, titanium, laser-weldable</b>	
J2253.0112	<b>Locator® Lab kits for extended angulation</b>	85		J2262.4300	Ø 3.3/3.8/4.3 mm	77
J2253.0200	<b>Locator® Impression cap</b>	84		J2262.6000	Ø 5.0 mm	77
J2253.0340	<b>Locator® Analog</b>	84			<b>Base for bar abutment, cast-on</b>	
J2253.0401	<b>Locator® Block out spacer</b>	85		J2263.4300	Ø 3.3/3.8/4.3 mm	77
J2253.0402	<b>Locator® Processing replacement male</b>	85		J2263.6000	Ø 5.0 mm	77
	<b>Locator® Replacement male</b>				<b>Aligning tool</b>	
J2253.1002	Ø 3.3/3.8/4.3/5.0 mm, blue, LOW	86		J2269.0005	17°	76
J2253.1003	Ø 3.3/3.8/4.3/5.0 mm, pink, MEDIUM	86		J2269.0006	30°	76
J2253.1005	Ø 3.3/3.8/4.3/5.0 mm, clear, HIGH	86			<b>Scanning cap for bar abutments</b>	
	<b>Locator® Replacement male for extended angulation</b>			J2610.4300	Ø 3.3/3.8/4.3 mm	76
J2253.2000	Ø 3.8/4.3/5.0 mm, gray, NO RETENTION	86		J2610.6000	Ø 5.0 mm	76
J2253.2002	Ø 3.8/4.3/5.0 mm, red, LOW	86			<b>Bar lab analog for bar abutments</b>	
J2253.2003	Ø 3.8/4.3/5.0 mm, orange, MEDIUM	86		J3020.4300	Ø 3.3/3.8/4.3 mm	76
J2253.2004	Ø 3.8/4.3/5.0 mm, green, HIGH	86		J3020.6000	Ø 5.0 mm	76
	<b>Crown base for bar abutment</b>				<b>Polishing protection for caps and bases for bar abutment</b>	
J2256.4306	Ø 3.3/3.8/4.3 mm	77		J3021.4300	Ø 3.3/3.8/4.3 mm	78
J2256.6006	Ø 5.0 mm	77		J3021.6000	Ø 5.0 mm	78
	<b>Base for bar abutment, burn-out</b>				<b>Handle for CAMLOG®/CONELOG® Implant analog</b>	
J2257.4301	Ø 3.3/3.8/4.3 mm	77		J3025.0010	Ø 3.3/3.8/4.3 mm	92
J2257.6001	Ø 5.0 mm	77		J3025.0015	Ø 5.0 mm	92
	<b>Base for bar abutment, solderable</b>				<b>Bar implant analog for bar abutments</b>	
J2258.4300	Ø 3.3/3.8/4.3 mm	77		J3025.4300	Ø 3.3/3.8/4.3 mm	76
J2258.6000	Ø 5.0 mm	77		J3025.6000	Ø 5.0 mm	76

# Index Article Number

	<b>Gingiva height indicator, straight</b>						
J3550.3300	Ø 3.3 mm	76		J5002.0011	Adapter, ISO shaft		53
J3550.3800	Ø 3.8 mm	76		J5002.0012	Cleaning needle		55
J3550.4300	Ø 4.3 mm	76		J5002.0013	Wrench adapter		36
J3550.5000	Ø 5.0 mm	76		J5002.0020	Cleaning cannula		55
J3551.0001	<b>Orientation gauge for COMFOUR®</b>	76					
J3709.0015	<b>Universal holder</b>	92			<b>Bone profiler</b>		
	<b>Reworking reamer, base for bar abutment</b>			J5003.3350	Ø 3.3 mm, Ø 5.0 mm		50
J3711.0010	Ø 3.3/3.8/4.3 mm, plane surface/cone seat	92		J5003.4360	Ø 3.8/4.3 mm, Ø 6.0 mm		50
J3711.0015	Ø 5.0 mm, plane surface/cone seat	92		J5003.5070	Ø 5.0 mm, Ø 7.0 mm		50
J3711.0020	Ø 3.3/3.8/4.3 mm, screw seat	92			<b>Baring drill for cover screw</b>		
J3711.0025	Ø 5.0 mm, screw seat	92		J5004.3300	Ø 3.3 mm		50
	<b>Guide System guiding sleeve</b>			J5004.3800	Ø 3.8 mm		50
J3734.3303	Ø 3.3 mm	47		J5004.4300	Ø 4.3 mm		50
J3734.3803	Ø 3.8 mm	47		J5004.5000	Ø 5.0 mm		50
J3734.4303	Ø 4.3 mm	47			<b>Countersink</b>		
	<b>Guide System guiding sleeve</b>			J5006.3346	Ø 3.3 mm, Ø 4.6 mm		50
	<b>PROGRESSIVE-LINE</b>			J5006.3852	Ø 3.8 mm, Ø 5.2 mm		50
J3754.3301	Ø 3.3 mm	32		J5006.4356	Ø 4.3 mm, Ø 5.6 mm		50
J3754.3801	Ø 3.8 mm	32		J5006.5063	Ø 5.0 mm, Ø 6.3 mm		50
J3754.4301	Ø 4.3 mm	32			<b>Depth stop SCREW-LINE for pilot drills and pre-drills</b>		
J3754.5001	Ø 5.0 mm	32		J5015.0009	L 9 mm		50
	<b>Plastic screw for bar abutment</b>			J5015.0011	L 11 mm		50
J4009.1627	M1.6	79		J5015.0013	L 13 mm		50
J4009.2027	M2.0	79			<b>Depth stop for form drills</b>		
	<b>Prosthetic screw for bar abutment</b>				<b>PROGRESSIVE-LINE and SCREW-LINE</b>		
J4012.1601	Ø 3.3/3.8/4.3 mm	78		J5015.3300	Ø 3.3 mm	25, 43	
J4012.2001	Ø 5.0 mm	78		J5015.3800	Ø 3.8 mm	25, 43	
	<b>Screw, hex</b>			J5015.4300	Ø 4.3 mm	25, 43	
J4012.1610	L 10 mm, M1.6	79		J5015.5000	Ø 5.0 mm	25, 43	
J4012.1615	L 15 mm, M1.6	79			<b>Guide System gingiva punch</b>		
J4012.1620	L 20 mm, M1.6	79		J5041.3303	Ø 3.3 mm		47
J4012.2010	L 10 mm, M2.0	79		J5041.3304	Ø 3.3 mm, PROGRESSIVE-LINE		31
J4012.2015	L 15 mm, M2.0	79		J5041.3803	Ø 3.8 mm		47
J4012.2020	L 20 mm, M2.0	79		J5041.3804	Ø 3.8 mm, PROGRESSIVE-LINE		31
	<b>Lab prosthetic screw for bar abutment</b>			J5041.4303	Ø 4.3 mm		47
J4013.1601	Ø 3.3/3.8/4.3 mm	78		J5041.4304	Ø 4.3 mm, PROGRESSIVE-LINE		31
J4013.2001	Ø 5.0 mm	78		J5041.5004	Ø 5.0 mm, PROGRESSIVE-LINE		31
	<b>Drill extension, ISO shaft</b>			J5050.2300	Round bur		49
J5002.0005	for instruments with internal irrigation	47		J5051.1500	Point drill		49
J5002.0006	not for drills with internal irrigation	51		J5051.2000	Pilot drill SCREW-LINE		49
				J5051.2003	Pilot drill		49
				J5051.2800	Pre-drill SCREW-LINE		49

	<b>Form drill SCREW-LINE cortical bone</b>				
J5053.3316	Ø 3.3 mm	43	J5063.3309	Ø 3.3 mm, L 5/9 mm	46
J5053.3816	Ø 3.8 mm	43	J5063.3311	Ø 3.3 mm, L 5/9/11 mm	46
J5053.4316	Ø 4.3 mm	43	J5063.3313	Ø 3.3 mm, L 5/9/11/13 mm	46
J5053.5016	Ø 5.0 mm	43	J5063.4307	Ø 3.8/4.3 mm, L 5/7 mm	46
	<b>Tap SCREW-LINE</b>		J5063.4309	Ø 3.8/4.3 mm, L 5/9 mm	46
J5054.3309	Ø 3.3 mm	43	J5063.4311	Ø 3.8/4.3 mm, L 5/9/11 mm	46
J5054.3809	Ø 3.8 mm	43	J5063.4313	Ø 3.8/4.3 mm, L 5/9/11/13 mm	46
J5054.4309	Ø 4.3 mm	43	J5064.3316	Ø 3.3 mm, L 16 mm	46
J5054.5009	Ø 5.0 mm	43	J5064.4316	Ø 3.8/4.3 mm, L 16 mm	46
J5060.0001	<b>EP pilot drill set</b>	44		<b>Guide System surgery set SCREW-LINE</b>	
J5060.2800	<b>SCREW-LINE EP pre-drill</b>	44	J5065.3309	Ø 3.3 mm, L 5/9 mm	46
	<b>SCREW-LINE EP form drill</b>		J5065.3311	Ø 3.3 mm, L 5/9/11 mm	46
J5060.3309	Ø 3.3 mm, L 9 mm	44	J5065.3313	Ø 3.3 mm, L 5/9/11/13 mm	46
J5060.3311	Ø 3.3 mm, L 11 mm	44	J5065.3807	Ø 3.8 mm, L 5/7 mm	46
J5060.3313	Ø 3.3 mm, L 13 mm	44	J5065.3809	Ø 3.8 mm, L 5/9 mm	46
J5060.3807	Ø 3.8 mm, L 7 mm	44	J5065.3811	Ø 3.8 mm, L 5/9/11 mm	46
J5060.3809	Ø 3.8 mm, L 9 mm	44	J5065.3813	Ø 3.8 mm, L 5/9/11/13 mm	46
J5060.3811	Ø 3.8 mm, L 11 mm	44	J5065.4307	Ø 4.3 mm, L 5/7 mm	46
J5060.3813	Ø 3.8 mm, L 13 mm	44	J5065.4309	Ø 4.3 mm, L 5/9 mm	46
J5060.4307	Ø 4.3 mm, L 7 mm	44	J5065.4311	Ø 4.3 mm, L 5/9/11 mm	46
J5060.4309	Ø 4.3 mm, L 9 mm	44	J5065.4313	Ø 4.3 mm, L 5/9/11/13 mm	46
J5060.4311	Ø 4.3 mm, L 11 mm	44	J5066.3316	Ø 3.3 mm, L 16 mm	46
J5060.4313	Ø 4.3 mm, L 13 mm	44	J5066.3816	Ø 3.8 mm, L 16 mm	46
J5060.5007	Ø 5.0 mm, L 7 mm	44	J5066.4316	Ø 4.3 mm, L 16 mm	46
J5060.5009	Ø 5.0 mm, L 9 mm	44		<b>Guide System Form drill, SCREW-LINE cortical bone</b>	
J5060.5011	Ø 5.0 mm, L 11 mm	44	J5068.3309	Ø 3.3 mm, L 9 mm	47
J5060.5013	Ø 5.0 mm, L 13 mm	44	J5068.3311	Ø 3.3 mm, L 11 mm	47
	<b>Form drill SCREW-LINE</b>		J5068.3313	Ø 3.3 mm, L 13 mm	47
J5062.3309	Ø 3.3 mm, L 9 mm	43	J5068.3316	Ø 3.3 mm, L 16 mm	47
J5062.3311	Ø 3.3 mm, L 11 mm	43	J5068.3807	Ø 3.8 mm, L 7 mm	47
J5062.3313	Ø 3.3 mm, L 13 mm	43	J5068.3809	Ø 3.8 mm, L 9 mm	47
J5062.3316	Ø 3.3 mm, L 16 mm	43	J5068.3811	Ø 3.8 mm, L 11 mm	47
J5062.3807	Ø 3.8 mm, L 7 mm	43	J5068.3813	Ø 3.8 mm, L 13 mm	47
J5062.3809	Ø 3.8 mm, L 9 mm	43	J5068.3816	Ø 3.8 mm, L 16 mm	47
J5062.3811	Ø 3.8 mm, L 11 mm	43	J5068.4307	Ø 4.3 mm, L 7 mm	47
J5062.3813	Ø 3.8 mm, L 13 mm	43	J5068.4309	Ø 4.3 mm, L 9 mm	47
J5062.3816	Ø 3.8 mm, L 16 mm	43	J5068.4311	Ø 4.3 mm, L 11 mm	47
J5062.4307	Ø 4.3 mm, L 7 mm	43	J5068.4313	Ø 4.3 mm, L 13 mm	47
J5062.4309	Ø 4.3 mm, L 9 mm	43	J5068.4316	Ø 4.3 mm, L 16 mm	47
J5062.4311	Ø 4.3 mm, L 11 mm	43			
J5062.4313	Ø 4.3 mm, L 13 mm	43			
J5062.4316	Ø 4.3 mm, L 16 mm	43			
J5062.5007	Ø 5.0 mm, L 7 mm	43			
J5062.5009	Ø 5.0 mm, L 9 mm	43			
J5062.5011	Ø 5.0 mm, L 11 mm	43			
J5062.5013	Ø 5.0 mm, L 13 mm	43			
J5062.5016	Ø 5.0 mm, L 16 mm	43			

# Index Article Number

	<b>Form drill PROGRESSIVE-LINE</b>				
J5070.3309	Ø 3.3 mm, L 9 mm	25			
J5070.3311	Ø 3.3 mm, L 11 mm	25			
J5070.3313	Ø 3.3 mm, L 13 mm	25			
J5070.3316	Ø 3.3 mm, L 16 mm	25			
J5070.3807	Ø 3.8 mm, L 7 mm	25			
J5070.3809	Ø 3.8 mm, L 9 mm	25			
J5070.3811	Ø 3.8 mm, L 11 mm	25			
J5070.3813	Ø 3.8 mm, L 13 mm	25			
J5070.3816	Ø 3.8 mm, L 16 mm	25			
J5070.4307	Ø 4.3 mm, L 7 mm	25			
J5070.4309	Ø 4.3 mm, L 9 mm	25			
J5070.4311	Ø 4.3 mm, L 11 mm	25			
J5070.4313	Ø 4.3 mm, L 13 mm	25			
J5070.4316	Ø 4.3 mm, L 16 mm	25			
J5070.5007	Ø 5.0 mm, L 7 mm	25			
J5070.5009	Ø 5.0 mm, L 9 mm	25			
J5070.5011	Ø 5.0 mm, L 11 mm	25			
J5070.5013	Ø 5.0 mm, L 13 mm	25			
J5070.5016	Ø 5.0 mm, L 16 mm	25			
	<b>Tap PROGRESSIVE-LINE</b>				
J5071.3300	Ø 3.3 mm	25, 36			
J5071.3800	Ø 3.8 mm	25, 36			
J5071.4300	Ø 4.3 mm	25, 36			
J5071.5000	Ø 5.0 mm	25, 36			
	<b>Dense bone drill PROGRESSIVE-LINE</b>				
J5072.3300	Ø 3.3 mm	25, 36			
J5072.3800	Ø 3.8 mm	25, 36			
J5072.4300	Ø 4.3 mm	25, 36			
J5072.5000	Ø 5.0 mm	25, 36			
	<b>Guide System pilot drill PROGRESSIVE-LINE</b>				
J5074.3305	Ø 3.3 mm, L 5 mm	31			
J5074.3309	Ø 3.3 mm, L 9 mm	31			
J5074.3311	Ø 3.3 mm, L 11 mm	31			
J5074.3313	Ø 3.3 mm, L 13 mm	31			
J5074.3316	Ø 3.3 mm, L 16 mm	31			
J5074.4305	Ø 3.8/4.3 mm, L 5 mm	31			
J5074.4307	Ø 3.8/4.3 mm, L 7 mm	31			
J5074.4309	Ø 3.8/4.3 mm, L 9 mm	31			
J5074.4311	Ø 3.8/4.3 mm, L 11 mm	31			
J5074.4313	Ø 3.8/4.3 mm, L 13 mm	31			
J5074.4316	Ø 3.8/4.3 mm, L 16 mm	31			
J5074.5005	Ø 5.0 mm, L 5 mm	31			
J5074.5007	Ø 5.0 mm, L 7 mm	31			
J5074.5009	Ø 5.0 mm, L 9 mm	31			
J5074.5011	Ø 5.0 mm, L 11 mm	31			
J5074.5013	Ø 5.0 mm, L 13 mm	31			
J5074.5016	Ø 5.0 mm, L 16 mm	31			
	<b>Guide System pre-drill PROGRESSIVE-LINE</b>				
J5076.3305	Ø 3.3 mm, L 5 mm	31			
J5076.3805	Ø 3.8 mm, L 5 mm	31			
J5076.4305	Ø 4.3 mm, L 5 mm	31			
J5076.5005	Ø 5.0 mm, L 5 mm	31			
	<b>Guide System form drill PROGRESSIVE-LINE</b>				
J5076.3309	Ø 3.3 mm, L 9 mm	31			
J5076.3311	Ø 3.3 mm, L 11 mm	31			
J5076.3313	Ø 3.3 mm, L 13 mm	31			
J5076.3316	Ø 3.3 mm, L 16 mm	31			
J5076.3807	Ø 3.8 mm, L 7 mm	31			
J5076.3809	Ø 3.8 mm, L 9 mm	31			
J5076.3811	Ø 3.8 mm, L 11 mm	31			
J5076.3813	Ø 3.8 mm, L 13 mm	31			
J5076.3816	Ø 3.8 mm, L 16 mm	31			
J5076.4307	Ø 4.3 mm, L 7 mm	31			
J5076.4309	Ø 4.3 mm, L 9 mm	31			
J5076.4311	Ø 4.3 mm, L 11 mm	31			
J5076.4313	Ø 4.3 mm, L 13 mm	31			
J5076.4316	Ø 4.3 mm, L 16 mm	31			
J5076.5007	Ø 5.0 mm, L 7 mm	31			
J5076.5009	Ø 5.0 mm, L 9 mm	31			
J5076.5011	Ø 5.0 mm, L 11 mm	31			
J5076.5013	Ø 5.0 mm, L 13 mm	31			
J5076.5016	Ø 5.0 mm, L 16 mm	31			
	<b>Guide System form drill for Ø 3.8 mm underpreparation PROGRESSIVE-LINE</b>				
J5077.3309	Ø 3.3 mm, L 9 mm	32			
J5077.3311	Ø 3.3 mm, L 11 mm	32			
J5077.3313	Ø 3.3 mm, L 13 mm	32			
J5077.3316	Ø 3.3 mm, L 16 mm	32			
	<b>Guide System dense bone drill PROGRESSIVE-LINE</b>				
J5078.3309	Ø 3.3 mm, L 9 mm	32			
J5078.3311	Ø 3.3 mm, L 11 mm	32			
J5078.3313	Ø 3.3 mm, L 13 mm	32			
J5078.3316	Ø 3.3 mm, L 16 mm	32			
J5078.3807	Ø 3.8 mm, L 7 mm	32			
J5078.3809	Ø 3.8 mm, L 9 mm	32			
J5078.3811	Ø 3.8 mm, L 11 mm	32			
J5078.3813	Ø 3.8 mm, L 13 mm	32			
J5078.3816	Ø 3.8 mm, L 16 mm	32			
J5078.4307	Ø 4.3 mm, L 7 mm	32			
J5078.4309	Ø 4.3 mm, L 9 mm	32			
J5078.4311	Ø 4.3 mm, L 11 mm	32			
J5078.4313	Ø 4.3 mm, L 13 mm	32			
J5078.4316	Ø 4.3 mm, L 16 mm	32			
J5078.5007	Ø 5.0 mm, L 7 mm	32			
J5078.5009	Ø 5.0 mm, L 9 mm	32			
J5078.5011	Ø 5.0 mm, L 11 mm	32			
J5078.5013	Ø 5.0 mm, L 13 mm	32			
J5078.5016	Ø 5.0 mm, L 16 mm	32			

	<b>Drill PROGRESSIVE-LINE Flex</b>								
J5079.3300	Ø 3.3 mm	36		J5300.8919	<b>Guide System surgery tray CAMLOG®/CONELOG® PROGRESSIVE-LINE (without contents)</b>				30
J5079.3800	Ø 3.8 mm	36							
J5079.4300	Ø 4.3 mm	36							
J5079.5000	Ø 5.0 mm	36							
	<b>Profile drill PROGRESSIVE-LINE Flex</b>			J5300.8968	<b>Surgery wash tray CAMLOG®/CONELOG®</b>				
J5080.3300	Ø 3.3 mm	36		J5300.8970	SCREW-LINE				42
J5080.3800	Ø 3.8 mm	36		J5300.8971	PROGRESSIVE-LINE				24
J5080.4300	Ø 4.3 mm	36			Guide System PROGRESSIVE-LINE				30
J5080.5000	Ø 5.0 mm	36							
J5300.0011	<b>Insertion tool for ball abutment</b>	88		J5302.0010	<b>Universal holding key</b>				54
	<b>Insertion tool for straight bar abutments</b>			J5302.3300	<b>Sleeve for inserting the insertion aid into the implant</b>				
J5300.0020	Ø 3.3/3.8/4.3 mm, short	88		J5302.3800	Ø 3.3 mm				54
J5300.0021	Ø 3.3/3.8/4.3 mm, long	89		J5302.4300	Ø 3.8 mm				54
J5300.0025	Ø 5.0 mm, short	88		J5302.5000	Ø 4.3 mm				54
					Ø 5.0 mm				54
J5300.0022	<b>Removal adapter for CAMLOG® and CONELOG®</b>	51							
	<b>Insertion tool for impression posts and healing caps for bar abutments</b>			J5317.0501	<b>Screwdriver, hex</b>				
J5300.0027	Ø 3.3/3.8/4.3 mm	76, 89		J5317.0502	short, manual/wrench				54, 90
J5300.0028	Ø 5.0 mm	76, 89		J5317.0503	long, manual/wrench				54, 90
				J5317.0503	long, ISO shaft				55, 91
J5300.0030	<b>PickUp instrument</b>	53		J5317.0504	short, ISO shaft				55, 91
	<b>Insertion tool for screw implants</b>			J5317.0510	extra short, manual/wrench				54, 90
J5300.0031	extra short, manual/wrench	52							
J5300.0032	short, manual/wrench	52		J5317.0511	<b>Manual screwdriver, hex</b>				55, 91
J5300.0033	long, manual/wrench	52		J5320.1030	<b>Torque wrench</b>				53, 88
J5300.0034	short, with ISO shaft for angled hand piece	52							
J5300.0035	long, with ISO shaft for angled hand piece	52		J5322.0010	<b>Tap adapter</b>				
	<b>Insertion tool for screw implants (without hex on shaft)</b>			J5322.0011	short				51
J5300.0036	short, with ISO shaft for angled hand piece	52			long				51
J5300.0037	long, with ISO shaft for angled hand piece	52		J5330.8500	<b>Prosthetic tray</b>				90
	<b>Surgery Set CAMLOG®/CONELOG®</b>			J5330.8700	<b>Prosthetic tray Universal</b>				90
J5300.0063	SCREW-LINE	42		J5417.2800	<b>Pre-osteotome SCREW-LINE, 1.7–2.8 mm, straight-convex</b>				57, 58
J5300.0065	PROGRESSIVE-LINE	24							
J5300.0071	PROGRESSIVE-LINE Flex	35		J5418.0020	<b>Osteotomy Set CAMLOG®/CONELOG® SCREW-LINE</b>				
	<b>Pattern for surgery wash tray CAMLOG®/CONELOG®</b>			J5418.0030	straight-convex				57
J5300.1072	Guide System PROGRESSIVE-LINE	30			angled-convex				58
J5300.1073	SCREW-LINE	42		J5418.3300	<b>Osteotome SCREW-LINE</b>				
J5300.1074	PROGRESSIVE-LINE	24		J5418.3310	Ø 3.3 mm, straight-convex				57
	<b>Paralleling pin</b>			J5418.3800	Ø 3.3 mm, angled-convex				58
J5300.2000	PROGRESSIVE-LINE	25		J5418.3810	Ø 3.8 mm, straight-convex				57
J5300.2028	SCREW-LINE	51		J5418.3810	Ø 3.8 mm, angled-convex				58
				J5418.4300	Ø 4.3 mm, straight-convex				57
				J5418.4310	Ø 4.3 mm, angled-convex				58
				J5418.5000	Ø 5.0 mm, straight-convex				57
				J5418.5010	Ø 5.0 mm, angled-convex				58

# Index Article Number

J5419.2800	<b>Pre-Osteotome SCREW-LINE, 1.7-2.8 mm, straight-concave</b>	59, 60
	<b>Osteotomy Set</b>	
	<b>CAMLOG®/CONELOG® SCREW-LINE</b>	
J5420.0020	straight-concave	59
J5420.0030	angled-concave	60
	<b>Osteotome SCREW-LINE</b>	
J5420.3300	Ø 3.3 mm, straight-concave	59
J5420.3310	Ø 3.3 mm, angled-concave	60
J5420.3800	Ø 3.8 mm, straight-concave	59
J5420.3810	Ø 3.8 mm, angled-concave	60
J5420.4300	Ø 4.3 mm, straight-concave	59
J5420.4310	Ø 4.3 mm, angled-concave	60
J5420.5000	Ø 5.0 mm, straight-concave	59
J5420.5010	Ø 5.0 mm, angled-concave	60
J8070.2050	<b>Edentulous mandible</b>	97





# Further documentation

**Further information on the CONELOG® Products can be found in the following documents:**

- CONELOG® Working Instructions
- CONELOG® Instructions for Use
- Preparation instructions
- Camlog literature overview
- Clinical evidence and Science

The documents are available from the local Camlog representative.

See also:

<https://ifu.camlog.com>

[www.camlog.com](http://www.camlog.com)

## References

- [1] Conserva E. Initial stability after placement of a new buttress-threaded implant. A case series study. *Implants*. 2019(3): 24-28.
- [2] Rupp J. One-year clinical experience with Progressive-Line implants. *EDI journal*. 2020(4): 54-63.
- [3] Semper-Hogg W, Kraft S, Stiller S, Mehrhof J, Nelson K. Analytical and experimental position stability of the abutment in different dental implant systems with a conical implant-abutment connection. *Clin Oral Investig*. 2013;17(3): 1017-23.
- [4] Semper-Hogg W, Zulauf K, Mehrhof J, Nelson K. The influence of torque tightening on the position stability of the abutment in conical implant-abutment connections. *Int J Prosthodont* 2015;28(5):538-41.

# Legal

## General disclaimer

The information provided is intended for marketing purposes only and does not qualify the user to use the product in a clinical setting. To ensure correct application, please refer to the relevant Instructions for Use and the Working Instructions before use.

## Trade names and Copyright

Protected trade names (trademarks) are not always specially indicated. The absence of such a reference does NOT mean that it is not a protected trademarked name. The document including all its parts is protected by copyright. You may download the content regarding the intended use, but changes to or reproduction of the content are not permitted. Any use outside the narrow limits of copyright law without the prior written consent of CAMLOG Biotechnologies GmbH is prohibited and is subject to legal sanctions.

CAMLOG®, COMFOUR®, CONELOG®, DEDICAM®, Esthomic®, Logfit® and Promote® are registered trademarks of CAMLOG Biotechnologies GmbH. Locator®, Locator R-Tx®, R-Tx, ZEST and Zest Dental Solutions, as well as the color and shape of the retention inserts are registered trademarks of ZEST IP Holdings, LLC.

The referenced trademarks may not be registered in all countries. All third party trademarks belong to the respective trademark owners. CAMLOG Biotechnologies GmbH can only place products on the market after approval by the competent national authorities. Therefore, not all products and services are available in all countries.

## Manufacturer

CAMLOG® and CONELOG® Products as well as all customized DEDICAM® Products are manufactured by:

ALTATEC GmbH | Maybachstr. 5 | 71299 Wimsheim | Germany

Locator® and Locator R-Tx® are manufactured by the Zest Anchors company.



**CE 0123**

Art. No. J8001.0009 Rev. 08 05/2023



+E219J800100091J



+S0080125505J\$

**Headquarters**

CAMLOG Biotechnologies GmbH | Margarethenstr. 38 | 4053 Basel | Switzerland  
Phone +41 61 565 41 00 | Fax +41 61 565 41 01 | info@camlog.com | www.biohorizonscamlog.com

Inspiring excellence in oral reconstruction

